


## OGT Handbook


---


### SureSeq Myeloid

### MRD 0.05% VAF Workflow



## Table of contents






## Introduction

---

This handbook describes the SureSeq™ Myeloid MRD 0.05% Workflow which has been developed and optimised for use with the SureSeq Myeloid MRD Panel designed by Oxford Gene Technology (OGT) to deliver accurate detection of a wide range of variants.

The OGT next-generation sequencing (NGS) range is compatible with Illumina NextSeq™ and NovaSeq™ chemistries.

There are sufficient reagents contained within the 96-reaction kit to process a total of 48 samples as a set of 8 samples on six occasions where 2 libraries are prepared per sample.



## Reagents, consumables and equipment

### Reagents supplied by OGT

Contents	Shipping/storage conditions	Cat. No. (96 reactions)
Universal Library Preparation Kit	Shipped at -20°C, store at -20°C	770100-96
Universal Index Adapters	Shipped at -20°C, store at -20°C	770200-96
Universal Hybridisation & Wash Kit V2	Shipped at -20°C, store at -20°C	770410-96
Pre-PCR Universal Bead Kit	Shipped at 4°C, store at 4°C	770310-96
Post-PCR Universal Bead Kit	Shipped at 4°C, store at 4°C	770315-96
SureSeq Myeloid MRD Panel	Shipped at -20°C, store at -20°C	770026-48

Universal Library Preparation Kit  
770100-96



Universal Index Adapters  
770200-96



Universal Hybridisation & Wash Kit V2  
770410-96



Pre-PCR Universal Bead Kit  
770310-96




Post-PCR Universal Bead Kit  
770315-96



SureSeq Myeloid MRD Panel  
770026-48






## Reagents, consumables and equipment

### Reagents supplied by user

Component	Suggested supplier	Cat. No.*
Molecular biology grade 100% ethanol	General laboratory supplier	–
Molecular biology grade water	General laboratory supplier	–
Molecular biology grade 5.0 M sodium hydroxide solution	General laboratory supplier	–
Qubit® dsDNA High Sensitivity (HS) Assay Kit	Thermo Fisher Scientific	Q32854
Qubit® dsDNA Broad Range (BR) Assay Kit	Thermo Fisher Scientific	Q32853
D1000 ScreenTape	Agilent Technologies	5067-5582
D1000 Reagents	Agilent Technologies	5067-5583
High Sensitivity D1000 ScreenTape	Agilent Technologies	5067-5584
High Sensitivity D1000 Reagents	Agilent Technologies	5067-5585
NextSeq 500/550 High-Output Kit v2.5 (300 cycles)	Illumina <sup>†</sup>	20024908
NextSeq 1000/2000 P2 Reagents (300 Cycles)	Illumina <sup>†</sup>	20046813
NovaSeq 6000 SP Reagent Kit v1.5 (300 cycles)	Illumina <sup>†</sup>	20028400
<i>Optional: Genomic DNA ScreenTape</i>	<i>Agilent Technologies</i>	<i>5067-5365</i>
<i>Optional: Genomic DNA Reagents</i>	<i>Agilent Technologies</i>	<i>5067-5366</i>

\* Catalogue numbers are correct for the UK; they may vary in other territories. For more information contact support@ogt.com

<sup>†</sup> Depending on sequencing device utilised.



## Reagents, consumables and equipment


### Consumables supplied by user

Component	Suggested supplier	Cat. No.*
Qubit Assay Tubes	Thermo Fisher Scientific	Q32856
DNA 1.5 ml LoBind® Tubes	Eppendorf	22431021
PCR Strips with attached Caps	Starlab	A1402-3700
Aerosol-resistant sterile pipette tips with filters 2, 10, 20, 200, 1000 µl	General laboratory supplier	-
<i>Optional: 15 ml or 50 ml Tubes</i>	<i>General laboratory supplier</i>	-
<i>Optional: Disposable reagent reservoirs</i>	<i>General laboratory supplier</i>	-

### Equipment supplied by user

Component	Stage required	Suggested supplier	Cat. No.*
Agilent® 4200 TapeStation®	Post-PCR	Agilent Technologies	G2991BA
2 x thermal cyclers (96-well) with heated lid	Pre- and Post-PCR	General laboratory supplier	-
Laboratory vortex mixer — OGT recommends IKA™ MS 3 Digital Vortex Mixer	Pre- and Post-PCR	IKA	IKA 0003319000
Plate adapter for vortex mixer — OGT recommends IKA MS 3.4 Microtiter Attachment	Post-PCR	IKA	IKA 0003426400
Microfuge for standard 1.5 ml tubes and 8-strip PCR tubes	Pre- and Post-PCR	General laboratory supplier	-
Magnet for 96-well microwell plate — OGT recommends DynaMag™-96 Side Magnet	Pre- and Post-PCR	Thermo Fisher Scientific	12331D
Magnet for 1.5 ml tubes — OGT recommends DynaMag-2 Magnet	Post-PCR	Thermo Fisher Scientific	12321D
Fluorometer (Qubit 4)	Pre- and Post-PCR	Thermo Fisher Scientific	Q33238
NanoDrop™ (One Microvolume UV-Vis Spectrophotometer)	Pre-PCR	Thermo Fisher Scientific	ND-ONE-W
20–200 µl and 1–10 µl 8-channel pipette	Pre- and Post-PCR	General laboratory supplier	-
Illumina NextSeq or NovaSeq	Post-PCR	Illumina	-

\* Catalogue numbers are correct for the UK; they may vary in other territories. For more information contact support@ogt.com



## General guidelines

---

### Recommended before you start

---



For best results, OGT recommends all steps are performed in PCR strip-tubes with attached caps.

It is highly recommended to test the hybridisation conditions (thermal cycler and plasticware) to ensure minimal evaporation occurs during the overnight incubation:

- To test, add 17  $\mu$ l of Nuclease-free Water (without DNA) in each well that you might use and use the thermal cycler settings in Table 9.
- Check after overnight incubation that the evaporation does not exceed 1–2  $\mu$ l per tube.
- If required, adjust the setting of the thermal cycler lids and/or use spacers appropriate to the model of thermal cycler.

Use fresh solution of 80% ethanol throughout the workflow using molecular biology grade ethanol and molecular biology grade water.

Where appropriate, allow the Mag-Bind<sup>®</sup> TotalPure NGS beads and the Dynabeads<sup>™</sup> M-270 Streptavidin magnetic beads to equilibrate to room temperature by removing them from their storage conditions at least 30 min before use.

### Storage and handling


---

The kit should be used before the expiry date indicated on the kit label.

The Universal Library Preparation Kit, Universal Index Adapters, SureSeq Myeloid MRD Panel and Universal Hybridisation & Wash Kit V2 should be stored at  $-20^{\circ}\text{C}$ .

The Pre-PCR and Post-PCR Universal Bead Kits should be stored at  $4^{\circ}\text{C}$ .





## General guidelines







### Safety

Handling of the SureSeq Myeloid MRD Panel should be carried out by trained laboratory staff in accordance with good laboratory practice, using the correct protective equipment such as laboratory coats, safety glasses and gloves.

The Universal Hybridisation & Wash Kit V2 contains chemicals that are potentially hazardous when mishandled. Particular care should be given to both Formamide and the Hybridisation Buffer.


Ensure that all operators have familiarised themselves with the safety data sheets (SDS) and relevant Risk Assessments before proceeding with the protocol.

### Symbols key

Symbol	Definition
	Important information: These notes are particularly important to read, understand and follow precisely.
	Time-saving tip: Optional suggestion to increase protocol efficiency.
	Cold step: Keep all components on ice for these steps.
	On-magnet step: Keep all tubes on magnet during these steps.
	Sequencing-specific information: These notes are particularly important to read, understand and follow precisely to optimally load the sequencing run.
	Safe stopping point: Samples can be safely stored at this stage without impacting results.

## Intended use

These products are for Research Use Only. The SureSeq Myeloid MRD 0.05% VAF Workflow is designed to be used by suitably trained personnel using DNA extracted from whole blood and/or bone marrow.



## Interpret NGS Analysis Software

Raw data FASTQ files with encoded UMIs generated from Illumina sequencers can be analysed using Interpret NGS Analysis Software and turned into interactive NGS analysis reports. The software is OGT's powerful, standalone data analysis package that is provided with the kit. For more information on how to generate the UMI FASTQ files, or any other software queries, contact your local OGT Field Application Specialist (FAS).

## Workflow overview

For ordering information about OGT products, visit [www.ogt.com](http://www.ogt.com).

The following section contains instructions for sample library production specific to the Illumina sequencing platform. In the SureSeq Myeloid MRD 0.05% VAF Workflow, each sample has two pre-hybridisation libraries prepared with the same index adapter. Each library pair is tagged with unique dual index (barcode) sequences, as well as unique molecular identifiers (UMI) for error correction and increased accuracy during analysis. Libraries are amplified and then pooled into sets of eight. Each pool is hybridised, captured and then amplified ready for sequencing.

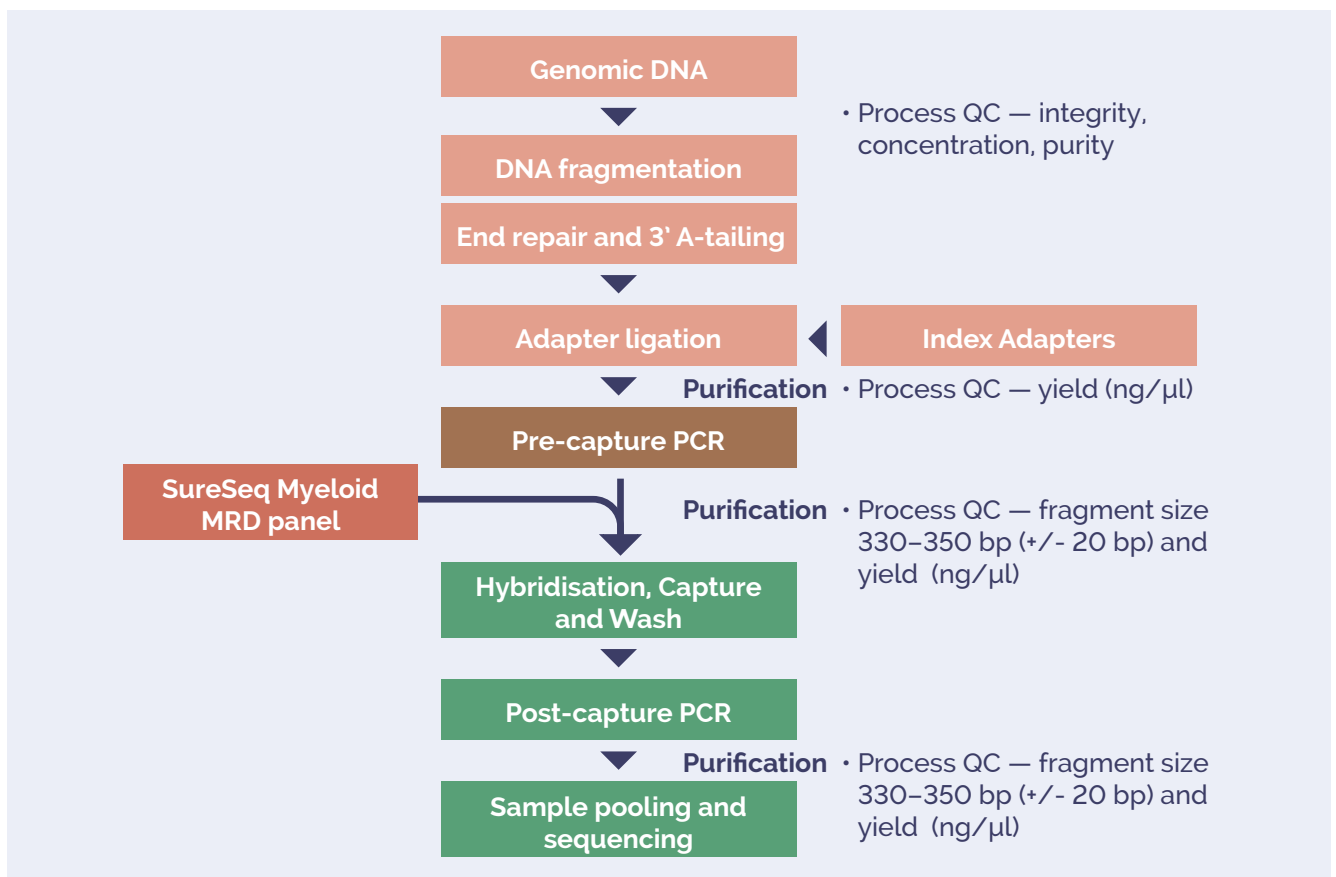


Figure 1: Workflow of sample library preparation indicating the expected DNA fragment size at each step of the procedure.

## Workflow overview


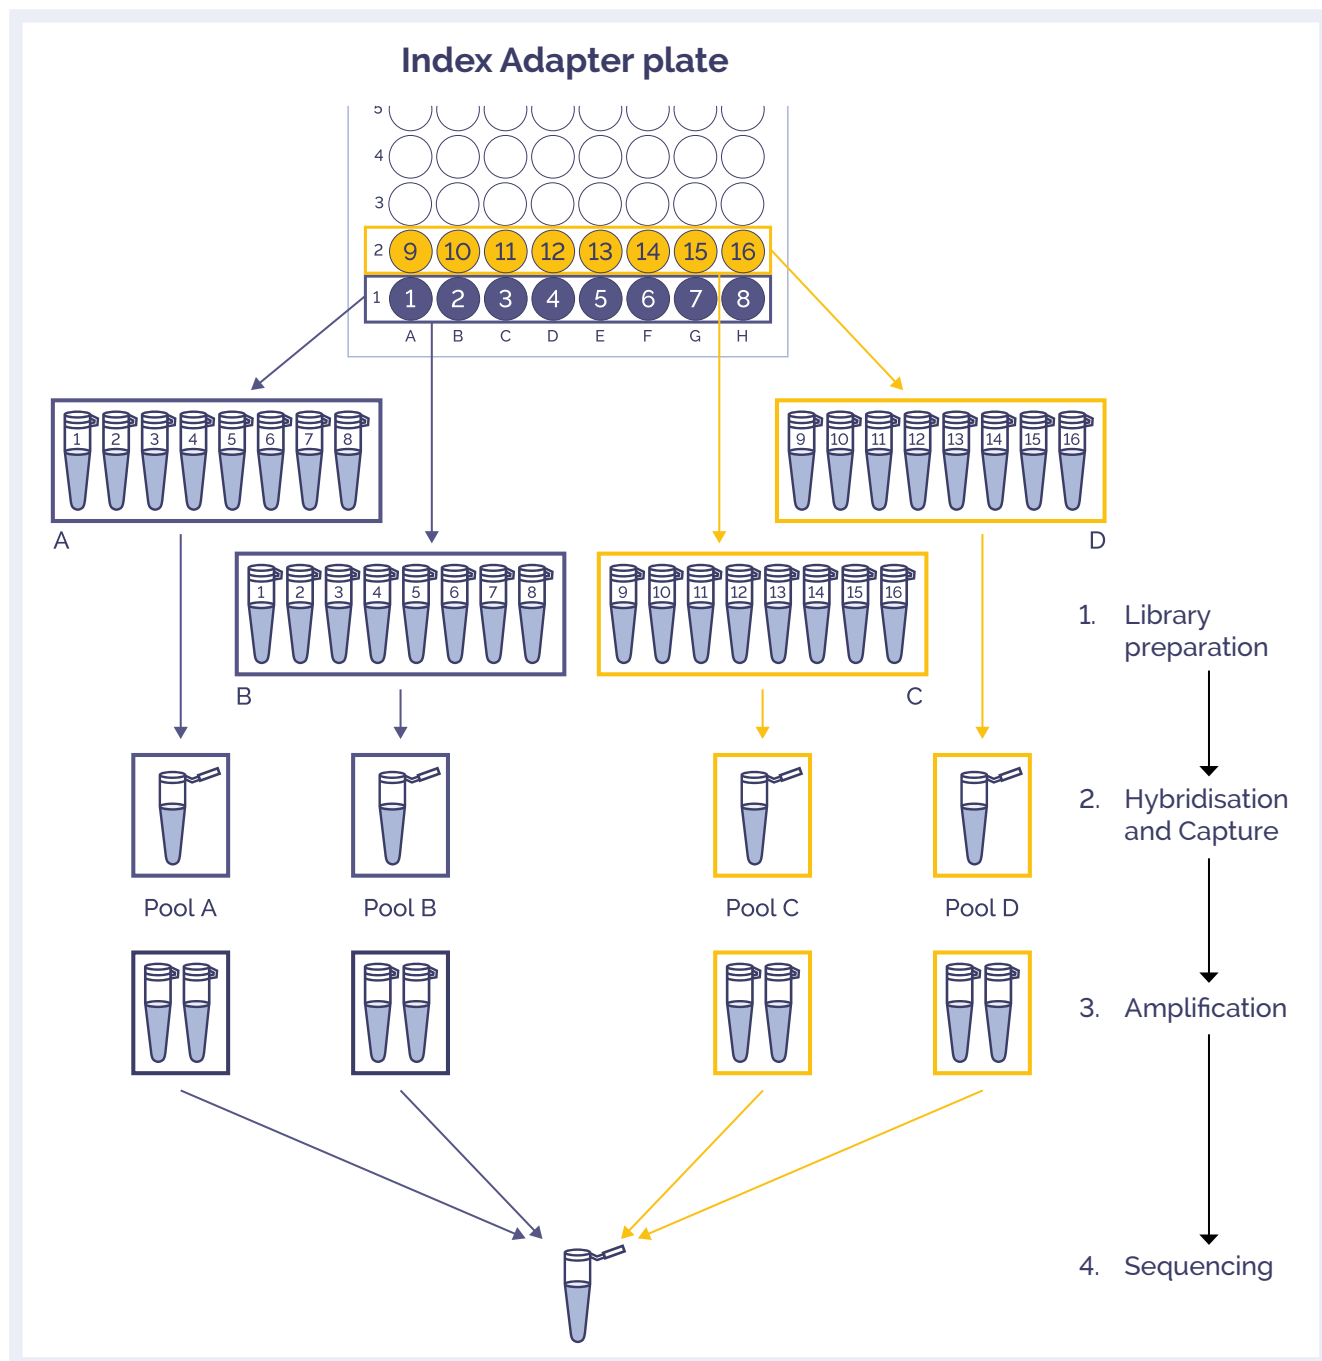


Figure 2: Outline of SureSeq Myeloid MRD 0.05% VAF Workflow for 16 samples.

1. Library preparation: 16 samples prepared in duplicate. Duplicates are ligated with the same Index Adapter.
2. Hybridisation: 4 pools, each consisting of one strip of eight libraries.
3. Post-capture PCR: 8 reactions prepared from duplicates of each hybridisation pool.
4. Sequencing: PCR reactions are pooled for sequencing.



## Sample requirements

### Sample requirements

The protocol has been optimised for a total DNA input of 400 ng per sample, split into two 200 ng replicates.



Modifying the recommended DNA input will impact downstream sequencing results.

### DNA — sample preparation

Determination of the concentration of gDNA sample is mandatory for all samples prior to starting the protocol.

DNA integrity and purity assessment are optional but recommended.

We recommend the following assays to assess the sample integrity, concentration and purity:

- Concentration: Thermo Fisher Scientific Qubit
- DNA integrity: Agilent 4200 TapeStation
- Purity: Thermo Scientific NanoDrop


### DNA concentration — Qubit dsDNA HS Assay Kit

Refer to manufacturer's user guide for the Thermo Fisher Scientific Qubit. The key steps are described below:

1. Prepare the Qubit working solution by diluting the Qubit reagent 1:200 in Qubit buffer.
2. Aliquot 190  $\mu$ l of Qubit working solution for the two standards.
3. Add 10  $\mu$ l of each Qubit standard to the appropriate tube.
4. Aliquot 199  $\mu$ l of Qubit working solution for each sample under assessment.
5. Add 1  $\mu$ l of sample to the appropriate tube.



Samples with an initial DNA concentration  $>100$  ng/ $\mu$ l should be prediluted to 20–100 ng/ $\mu$ l with TE Buffer (provided in the kit). Confirm the DNA concentration using the Qubit dsDNA HS Assay Kit. The precise quantification of DNA input is essential for reproducible fragmentation results.



## Sample requirements

---

6. Mix by vortexing for 2–3 sec, being careful not to generate bubbles.
7. Incubate the tubes at room temperature for 2 min.
8. Measure and record DNA concentrations following the onscreen prompts.

## DNA integrity — Genomic DNA ScreenTape

---

**Optional:** This step is important to assess the level, if any, of DNA degradation.

Refer to the manufacturer's user guide for the Agilent 4200 TapeStation. The key steps are described below:


1. Prepare the ladder by mixing 10  $\mu$ l of Genomic DNA Sample Buffer with 1  $\mu$ l Genomic DNA ladder in the first tube/well of the strip tube or plate.

**Note:** A ladder is required for each run. No electronic ladder is available for the Genomic DNA assay

2. For each sample under assessment, add 1  $\mu$ l of DNA sample to 10  $\mu$ l of Sample Buffer.
3. Seal all the tubes/wells.
4. Vortex the tubes or plate for 1 min at 2000 rpm and then briefly centrifuge to collect liquid at the bottom.
5. Briefly spin down to collect the sample at the bottom of the tubes/wells.
6. Load the strip of tubes or plate into the Agilent 4200 TapeStation.

**Note:** If using strip tubes remember to take off the caps.

7. Highlight the required samples on the controller software and fill in the sample names in the sample sheet.
8. Provide a filename in the "Prefix" field of the controller software to save your results and select "Start".



## Sample requirements

---

9. Check that the electropherogram shows that the integrity of the gDNA is intact with an even distribution and maximum peak size >5000 bp.
10. After DNA electrophoresis using the Agilent 4200 TapeStation, a DNA Integrity Number (DIN) is generated. A DIN >7 indicates the presence of intact DNA, while a DIN <7 indicates that the DNA is degraded. If a sample has a DIN <7 contact your local FAS.

## Purity — NanoDrop

---

**Optional:** This step is important to assess the purity of the DNA sample.


Refer to the manufacturer's user guide for the NanoDrop.

The key steps are described below:

1. Use the “Nucleic Acid” and “DNA-50” setting.
2. Clean the pedestal with Nuclease-free Water.
3. Load 1–2 µl of sample buffer or blanking solution.
4. Click “Measure blank”.
5. Clean the pedestal with a lint-free wipe.
6. Load 1–2 µl of each sample onto the pedestal.
7. Click “Measure”.
8. Record the readings for 260/230, 260/280 and the concentration (ng/µl).

An OD 260/280 ratio of 1.8 to 2.0 and OD 260/230 ratio of 2.0 to 2.2 is recommended. Use of DNA samples with lower ratios may result in poor performance.


Contact your local OGT Field Application Specialist (FAS) if you require any advice as to the quality of your samples.



## Library preparation: Step 1

### DNA fragmentation, end repair and 3' end A-tailing

#### Genomic DNA

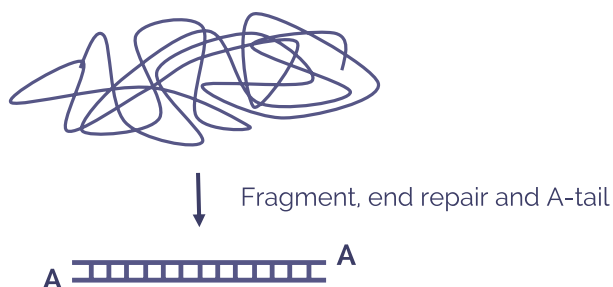

#### Overview

Genomic DNA is enzymatically fragmented. The fragmented dsDNA is repaired with enzymes in the Fragmentation and end repair (ER) mix to create blunt ends. At the same time, a 3' adenine overhang is created in preparation for adapter ligation.



It is recommended to process no more than 16 samples (32 libraries) in a single set up during the fragmentation step.

#### Before starting:


- ❄️ Remove TE Buffer (blue lid; ●) from storage ( $-15^{\circ}\text{C}$  to  $-25^{\circ}\text{C}$ ). Allow to thaw to room temperature then place on ice.



Use only the TE Buffer (blue lid; ●) provided in the kit for preparation of DNA samples (10 mM Tris, 1 mM EDTA). Use of other TE formulations (e.g., 0.1x TE) or water may affect fragmentation results.

- ❄️ Remove Step 1: Frag + ER Buffer (orange lid; ●) from storage ( $-15^{\circ}\text{C}$  to  $-25^{\circ}\text{C}$ ). Allow to thaw to room temperature and place on ice. Ensure that all components in the buffer are dissolved.

It is not uncommon to see precipitation in the buffer. If this occurs, pipette the buffer several times to break up the precipitate, followed by a quick vortex to mix until dissolved. If precipitate remains, then avoid pipetting precipitates into the Master Mix.



## Library preparation: Step 1

- ❄ • Remove Step 1: Frag + ER Enzyme (orange lid; ●) from storage ( $-15^{\circ}\text{C}$  to  $-25^{\circ}\text{C}$ ) and place on ice.
- Ensure DNA sample(s) are prediluted to 20–100 ng/ $\mu\text{l}$  with TE Buffer (blue lid; ●).

### Perform step 1: DNA fragmentation, end repair and 3' end A-tailing

Estimated time: 1.25 hr for 8–16 samples. Hands-on time: 15 min.

1. Program the thermal cycler using the settings shown in Table 1. Save the program as “OGT Fragmentation”.

Step	Temperature ( $^{\circ}\text{C}$ )	Time
1	37	20 min
2	65	30 min
3	4	Hold


Table 1: Incubation profile of program “OGT Fragmentation”

2. **Preheat** the thermal cycler to  $37^{\circ}\text{C}$ . Where possible, set the heated lid to  $75^{\circ}\text{C}$ , alternatively, have the pre-set heated lid activated.
- ❄ 3. In PCR strip-tubes, dilute **400 ng** of sample DNA with the chilled TE Buffer (blue lid; ●) provided to a total volume of **54  $\mu\text{l}$** . Mix on a vortex mixer for **3–5 sec**, pulse spin to collect the contents and place on ice.



Recommendation: prepare the samples as shown in Figure 3. This format will minimise pipetting steps during the Adapter ligation step.





## Library preparation: Step 1

- ❄️ 4. Label two new sets of PCR strip-tubes for each sample as shown in Figure 3 and place on ice.

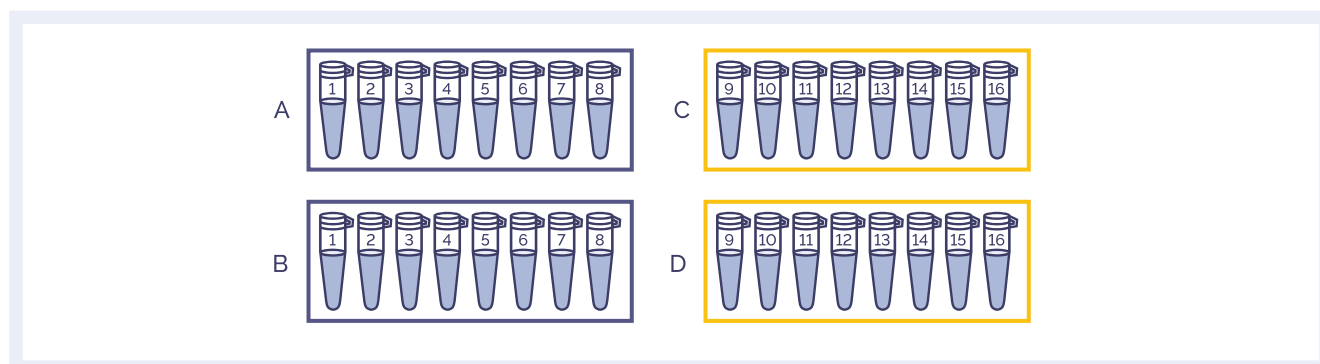


Figure 3: Recommended configuration for 16 samples. A/B and C/D indicate replicate strips and numbers indicate unique sample numbers.

- ❄️ 5. Mix Step 1: Frag + ER Buffer and Step 1: Frag + ER Enzyme on a vortex mixer for **5–8 sec**, pulse spin to collect the contents and place on ice.




It is essential to thoroughly mix the Frag + ER Enzyme for optimal performance.

- ❄️ 6. Prepare the Fragmentation and ER Master Mix according to Table 2 in a fresh 1.5 ml LoBind tube and place on ice.

Reagent	1x library (µl)	8x sample 16x library (µl) (includes 2 excess)	16x sample 32x library (µl) (includes 3 excess)
DNA sample	27	–	–
Step 1: Frag + ER Buffer (orange lid; ●)	7	126	245
Step 1: Frag + ER Enzyme (orange lid; ●)	1	18	35
<b>TOTAL</b>	<b>35</b>	<b>144</b>	<b>280</b>

Table 2: Fragmentation and ER Master Mix.

- ❄️ 7. Mix the Fragmentation and ER Master Mix on a vortex mixer for **3–5 sec**, pulse spin to collect the contents and keep on ice.



## Library preparation: Step 1

---

- ❄ 8. Add **8 µl** Fragmentation and ER Master Mix into each of the prepared empty tubes from step 4 and keep on ice.
- ❄ 9. Using a multi-channel pipette, add **27 µl** of DNA sample from step 3 to the tubes from step 4.



Proceed in a timely manner to avoid over-fragmentation as the enzyme is active at room temperature. Keep samples on ice when not being vortexed or spun.

10. **Immediately** mix on a vortex mixer for **3 sec**.
11. Pulse spin to collect the contents and **immediately** transfer to the **preheated** thermal cycler. Start the program “OGT Fragmentation”.




Recommendation: prepare the Ligation Master Mix in the final 10 minutes of the thermal cycler program.

12. When the program is complete and the thermal cycler has reached 4°C, remove the samples and place them on ice until you are ready to proceed with Adapter ligation.




We recommend continuing with “Step 2: Adapter ligation and purification” immediately. If necessary, samples can be stored at -20°C; however, a loss in yield (~20%) may be observed.



## Library preparation: Step 2

### Adapter ligation and purification


#### Overview

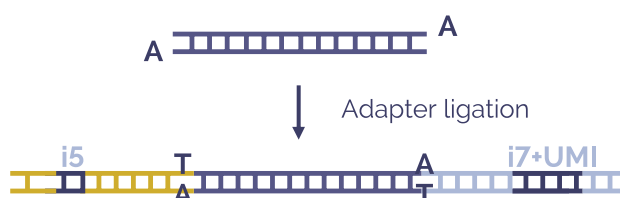

*Illumina compatible Adapter sequences are ligated onto the repaired dsDNA fragments with DNA ligase, using the 3' overhang created during end repair/A-tailing. Adapters contain unique molecular identifier (UMI) sequences and unique sample indexes.*

#### Before starting:

- Take the Mag-Bind TotalPure NGS beads from the Pre-PCR Universal Bead Kit out of the fridge at least **30 min before use** to allow them to warm to room temperature.
- Make up a fresh solution of 80% ethanol using molecular biology grade ethanol and molecular biology grade water.
- Remove the Step 2: Ligation Buffer (yellow lid; ●) from storage (–15°C to –25°C) and thaw to room temperature. Ensure that all components in the Ligase Buffer are well dissolved. If necessary, incubate at 37°C until dissolved.
- ❄ • Remove the Step 2: Ligase (yellow lid; ●) from storage (–15°C to –25°C) and place on ice.
- ❄ • Remove the Universal Index Adapter plate from storage (–15°C to –25°C) and allow to thaw on ice **5–10 min before use**. Pulse spin the Adapter plate in a centrifuge to collect the contents. Keep the plate on ice at all times. Do not heat above room temperature.
- Index Adapters are for single use only. If only using part of the plate, cover the used Adapter wells to avoid spillage of excess Index Adapter. Unused Adapters can also be aliquoted into strip tubes and thawed immediately prior to use.



## Library preparation: Step 2

- Assign a different Index Adapter to each library pair. See Figure 5 for the location of the Index Adapters on the plate.
- OGT recommends processing in batches of eight samples, each pool will contain a complete column from the index plate.

### Perform Step 2: Ligation

Estimated time: 35 min for 8–16 samples. Hands-on time: 15 min.

1. Program the thermal cycler using the settings shown in Table 3. Save the program as “OGT Ligation”.



Do not use heated lid. If heated lid cannot be turned off, keep lid open.

Step	Temperature (°C)	Time
1	20	20 min
2	4	Hold

Table 3: Incubation profile of program “OGT Ligation”

2. Mix Step 2: Ligase Buffer on a vortex mixer for **3–5 sec**, pulse spin to collect the contents and place on ice.
3. Flick mix Step 2: Ligase, pulse spin to collect the contents and place on ice.
4. Prepare the Ligation Master Mix according to Table 4 in a fresh 1.5 ml LoBind tube and place on ice..

Reagent	1x library (µl)	8x sample 16x library (µl) (includes 2 excess)	16x sample 32x library (µl) (includes 3 excess)
DNA sample	35	–	–
Index Adapter	2.5	–	–
Step 2: Ligase Buffer (yellow lid; ●)	9	162	315
Step 2: Ligase (yellow lid; ●)	2	36	70
<b>TOTAL</b>	<b>48.5</b>	<b>198</b>	<b>385</b>

Table 4: Ligation Master Mix.

## Library preparation: Step 2

- ❄ 5. Mix the Ligation Master Mix on a vortex mixer for **3–5 sec**, pulse spin to collect the contents and keep on ice.
- ❄ 6. Add **11  $\mu$ l** of the Ligation Master Mix to each chilled DNA sample tube containing the fragmented product(s).
7. Add **2.5  $\mu$ l** Index Adapter to each DNA sample tube from Step 5. Ensure the same Index Adapter is used for both replicates of a sample (see Figure 4).


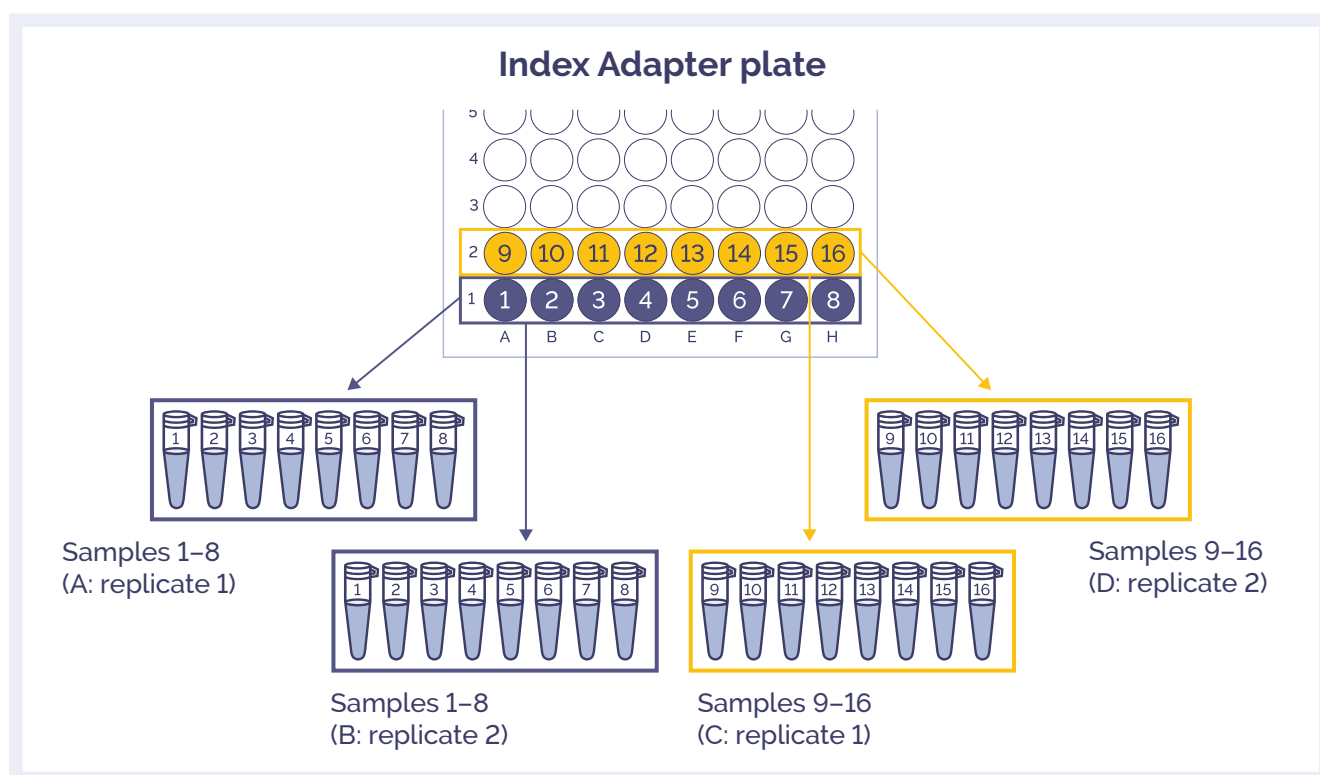


Figure 4: Pipetting scheme used when adding Index Adapter to DNA sample tubes. Duplicate strips are ligated with the same Index Adapter.

8. Mix on a vortex mixer for **3–5 sec** and pulse spin to collect the contents.
9. **Immediately** transfer to the thermal cycler and start the program “OGT Ligation”.
10. When the program is complete and the thermal cycler has reached 4°C, remove the samples and **proceed immediately** to “Ligated library purification”.



## Library preparation: Step 2

	1	2	3	4	5	6	7	8	9	10	11	12
A	1	9	17	25	33	41	49	57	65	73	81	89
B	2	10	18	26	34	42	50	58	66	74	82	90
C	3	11	19	27	35	43	51	59	67	75	83	91
D	4	12	20	28	36	44	52	60	68	76	84	92
E	5	13	21	29	37	45	53	61	69	77	85	93
F	6	14	22	30	38	46	54	62	70	78	86	94
G	7	15	23	31	39	47	55	63	71	79	87	95
H	8	16	24	32	40	48	56	64	72	80	88	96

Figure 5: Layout of Universal Index Adapter Plate (1–96).

### Perform Ligated library purification


Estimated hands on time: 50 min for 8–16 samples.



Prior to use, mix beads on a vortex mixer for at least 1 min or until the bead solution appears homogeneous and consistent in colour.

#### Before starting:

1. Prepare **two new** sets of fresh PCR strip-tubes for each strip of libraries. 16 samples (32 libraries) will require 8 strips of 8 tubes.
2. To the first set of tubes, add **51.5 µl** of Nuclease-free Water and **22 µl** of homogeneous, room temperature Mag-Bind TotalPure NGS beads from the Pre-PCR Universal Bead Kit and set aside until required in Step 4.



## Library preparation: Step 2

- To the second set of tubes, add **58  $\mu$ l** of homogeneous, room temperature Mag-Bind TotalPure NGS beads from the Pre-PCR Universal Bead Kit and set aside until required in Step 7.

### To the DNA sample tubes:

- Transfer the samples to the first set of tubes containing water and beads prepared in Step 2. Mix on a vortex mixer to resuspend the beads and pulse spin to collect the contents.
- Incubate at room temperature for **5 min.**




- Place the tubes in the magnetic stand and wait for the solution to clear (approx. 3–5 min).
- Transfer **120  $\mu$ l** of **cleared supernatant containing the DNA sample** to the second set of tubes containing beads prepared in Step 3. The used bead pellets can be discarded.
- Mix on a vortex mixer to resuspend the beads and pulse spin to collect the contents.
- Incubate at room temperature for **5 min.**



- Place the tubes in the magnetic stand and wait for the solution to clear (approx. 3–5 min).
- Avoiding the bead pellet, remove and discard the cleared supernatant (~180  $\mu$ l). **Keep the beads containing the DNA sample.**
- Add **200  $\mu$ l** of 80% ethanol to each tube without resuspending the bead pellet.
- Incubate for **30 sec**, then remove the ethanol.
- Repeat wash (Steps 12 and 13) once, for a total of two washes.
- Seal the tubes and pulse spin to collect the residual ethanol. Return the tubes to the magnetic stand. Remove the residual ethanol with a P20 pipette.
- Dry the bead pellets at room temperature for **1–2 min.**



Do not over-dry as this will decrease yield. The bead pellet is dry when the appearance of the surface changes from shiny to matt. Over-drying results in cracks in the bead pellet.



## Library preparation: Step 2

17. Remove from the magnetic stand and add **34  $\mu$ l** of Nuclease-free Water directly to the bead pellet to elute the DNA sample. Mix on a vortex mixer to resuspend the beads and pulse spin to collect the contents.
18. Incubate for **5 min** at room temperature.



Recommendation: If proceeding with Step 3: Pre-capture PCR immediately, the Step 3: Primer Mix and Step 3: PCR Buffer can be removed from storage to thaw to room temperature now.

19. Label a new set of PCR strip-tubes for the libraries and set aside until required in Step 21.




20. Place the tubes on the magnetic stand and wait for the solution to clear (approx. 2–3 min).
21. Transfer **32  $\mu$ l** of the eluate containing the purified ligated products to the tubes from Step 19. Tubes containing beads can be discarded at this time.
22. Assess yield using **1  $\mu$ l** ligated product with the Qubit dsDNA HS Kit as per manufacturer's instructions. The expected yield is  $>2$  ng/ $\mu$ l.



**OPTIONAL STOPPING POINT:** If the samples are not to be used immediately, store at  $-20$  °C. If continuing, proceed to "Pre-capture PCR".






## Library preparation: Step 3

### Pre-capture PCR


#### Overview

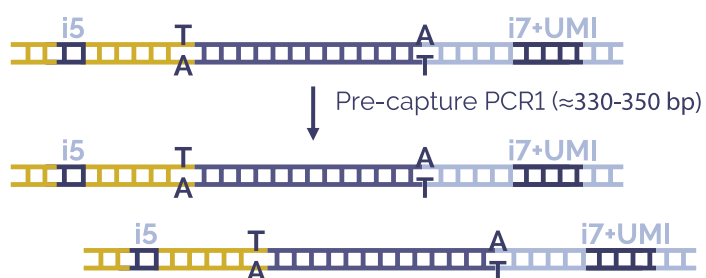

High fidelity PCR is used to amplify the DNA library prior to hybridisation and target capture. The number of PCR cycles is to be kept to a minimum to reduce the number of duplicate reads (PCR copies of the same original DNA fragment) in the sequencing data.

#### Before starting:

- Remove the Step 3: Primer Mix (red lid; ●) and Step 3: PCR Buffer (red lid; ●) from storage ( $-15^{\circ}\text{C}$  to  $-25^{\circ}\text{C}$ ) and allow to thaw at room temperature.
- Ensure that all components in the PCR Buffer are well dissolved. If necessary vortex mix and/or incubate at  $37^{\circ}\text{C}$  until dissolved.
- ❄ • Remove the Step 3: PCR Polymerase (red lid; ●) from storage ( $-15^{\circ}\text{C}$  to  $-25^{\circ}\text{C}$ ) and place on ice.



## Library preparation: Step 3

### Perform step 3: Pre-capture PCR


Estimated time: 45 min for 8–16 samples. Hands-on time: 15 min.

1. Program the thermal cycler using the settings shown in Table 5. Save the program as “OGT PCR1”. Where possible, set the heated lid to 105°C, alternatively have the pre-set heated lid activated.

Step	Temperature (°C)	Time
1	98	3 min
2	98	30 sec
3	65	30 sec
4	72	1 min
5	Repeat Step 2 to Step 4 for a total number of 6 cycles.	
6	72	10 min
7	4	Hold

Table 5: Incubation profile of program “OGT PCR1”.

2. Vortex Step 3: Primer Mix and Step 3: PCR Buffer on a vortex mixer for **3–5 sec** and pulse spin to collect the contents.
- ❄️ 3. Flick mix Step 3: PCR Polymerase, pulse spin to collect the contents and keep on ice.



## Library preparation: Step 3

4. Prepare the Pre-capture PCR Master Mix according to Table 6 in a fresh 1.5 ml LoBind tube.

Reagent	1x library (µl)	8x sample 16x library (µl) (includes 2 excess)	16x sample 32x library (µl) (includes 3 excess)
Adapter-ligated DNA sample	31	–	–
Nuclease-free Water (clear lid ○)	9.5	171	332.5
Step 3: PCR Buffer (red lid; ●)	5	90	175
Step 3: Primer Mix (red lid; ●)	2.5	45	87.5
Step 3: PCR Polymerase (red lid; ●)	2	36	70
<b>TOTAL</b>	<b>50</b>	<b>342</b>	<b>665</b>

Table 6: Pre-capture PCR Master Mix.


5. Mix the Pre-capture PCR Master Mix on a vortex mixer for **3–5 sec** and pulse spin to collect the contents.
6. Add **19 µl** of the Pre-capture PCR Master Mix to each DNA sample tube containing the ligated products.
7. Mix on a vortex mixer for **3–5 sec** and pulse spin to collect the contents.
8. Transfer to the thermal cycler and start the program “OGT PCR1”.

### Perform pre-capture PCR purification

Estimated hands-on time: 40 min for 8–16 samples.






Prior to use, mix beads on a vortex mixer for at least 1 min or until the bead solution appears homogeneous and consistent in colour.



## Library preparation: Step 3

### To the DNA sample tubes:

1. Add **45  $\mu$ l** of homogeneous, room temperature Mag-Bind TotalPure NGS beads from the Post-PCR Universal Bead Kit to each DNA sample tube. Mix on a vortex mixer to resuspend the beads and pulse spin to collect the contents.
  2. Incubate at room temperature for **5 min**.
  3.  Place the tubes in the magnetic stand and wait for the solution to clear (approx. 3–5 min).
  4. Avoiding the bead pellet, remove and discard the cleared supernatant (**~90  $\mu$ l**). **Keep the beads containing the DNA sample.**
  5. Add **200  $\mu$ l** of 80% ethanol to each tube without resuspending the bead pellet.
  6. Incubate for **30 sec**, then remove the ethanol.
  7. Repeat wash (Step 5 and Step 6) once, for a total of two washes.
  8. Seal the tubes and pulse spin to collect the residual ethanol. Return the tubes to the magnetic stand. Remove the residual ethanol with a P20 pipette.
  9. Dry the bead pellets at room temperature for **1–2 min**.
-  Do not over-dry as this will decrease yield. The bead pellet is dry when the appearance of the surface changes from shiny to matt. Over-drying results in cracks in the bead pellet.
10. Remove from the magnetic stand and add **25  $\mu$ l** of Nuclease-free Water directly to the bead pellet to elute the DNA sample. Mix on a vortex mixer to resuspend the beads and pulse spin to collect the contents.
  11. Incubate for **5 min** at room temperature.
  12. Label a new set of PCR strip-tubes for the samples and set aside until required in Step 14.
  13.  Place the tubes on the magnetic stand and wait for the solution to clear (approx. 2–3 min).
  14. Transfer **24  $\mu$ l** of the eluate containing the purified amplified products to the tubes from Step 12. Tubes containing beads can be discarded at this time.

## Library preparation: Step 3

- Assess the size of the amplified product using the Agilent D1000 ScreenTape System. The electropherogram should show a peak size of 330–350 bp ( $\pm 20$  bp) (Figure 6). Set up the instrument and prepare the tape, samples and ladder following the manufacturer's instructions.

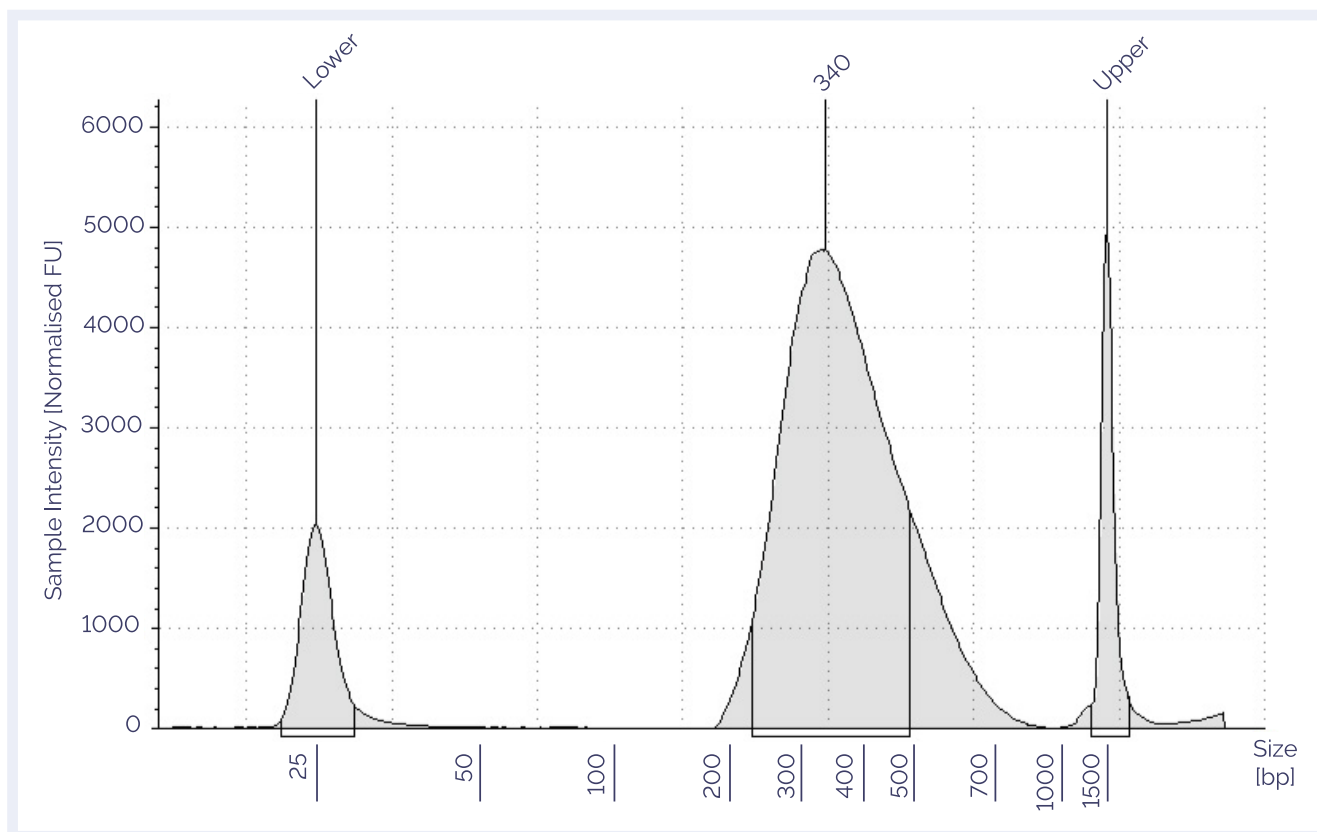


Figure 6: Electropherogram of purified Pre-capture PCR product generated using an Agilent D1000 ScreenTape assay. The electropherogram shows a maximum peak in the size range of approximately 330–350 bp ( $\pm 20$  bp).



Fragment sizes outside of this range may reduce sequence data quality. Contact your local Field Application Specialist (FAS) if you require further advice.


- Assess yield using **1  $\mu$ l** amplified product with the Qubit dsDNA HS Kit as per manufacturer's instructions.  
The expected yield is  $>18$  ng/ $\mu$ l ( $\sim 400$  ng per library).



It is recommended to use a single channel pipette and ensure there is no excess liquid on the side of the tip to prevent inaccurate readings affecting pooling.




**OPTIONAL STOPPING POINT:** If the samples are not to be used immediately, store at 4°C overnight or at  $-20^{\circ}\text{C}$  for long-term storage. If continuing, proceed to "Universal hybridisation".



## Library preparation: Universal hybridisation

### Universal hybridisation


#### Overview

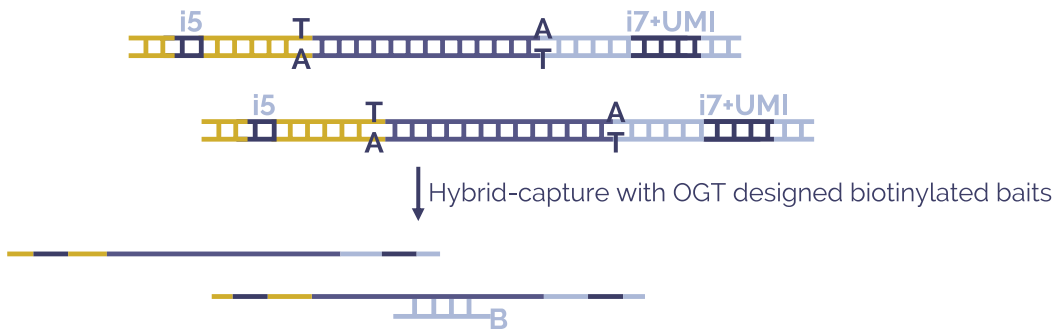

The amplified library is denatured and captured by SureSeq Biotinylated (B) baits.

#### Before starting:

- Take the Mag-Bind TotalPure NGS beads from the Post-PCR Universal Bead Kit out of the fridge at least **30 min before use** to allow them to warm to room temperature.
- Make up a fresh solution of 80% ethanol using molecular biology grade ethanol and molecular biology grade water.
- Remove the Hybridisation Buffer (red lid; ●), Formamide (yellow lid; ●), Cot Human DNA (green lid; ●), Index Blockers (blue lid; ●) and Nuclease-free Water (clear lid; ○) from storage ( $-15^{\circ}\text{C}$  to  $-25^{\circ}\text{C}$ ) and allow to thaw to room temperature.
- Remove the SureSeq Myeloid MRD Panel from storage ( $-15^{\circ}\text{C}$  to  $-25^{\circ}\text{C}$ ) and allow to thaw to room temperature.
- Ensure that all components in the Hybridisation Buffer are well dissolved. If necessary, incubate at  $37^{\circ}\text{C}$  until dissolved.



## Library preparation: Universal hybridisation

### Preparation of Hybridisation Master Mix

Estimated time: 5 min for 8–16 samples. Hands-on time: 5 min.

1. Mix Hybridisation Buffer, Formamide, Cot Human DNA, Myeloid MRD Panel and Index Blockers on a vortex mixer for **3–5 sec** and pulse spin to collect the contents.
2. Prepare the Hybridisation Master Mix according to Table 7 in a fresh 1.5 ml LoBind tube.

Reagent	1x Pool (µl)	2x Pool (µl) (includes 0.5 excess)	4x Pool (µl) (includes 0.5 excess)
Nuclease-free Water (clear lid; ○)	2.5	6.25	11.25
Hybridisation Buffer (red lid; ●)	7.5	18.75	33.75
Formamide (yellow lid; ●)	3.5	8.75	15.75
<b>TOTAL</b>	<b>13.5</b>	<b>33.75</b>	<b>60.75</b>

Table 7: Hybridisation Master Mix.

3. Mix on a vortex mixer and pulse spin to collect the contents.
4. **Proceed immediately** to “Pool samples and hybridise to capture baits”.

### Pool samples and hybridise to capture baits

Estimated time: 40 min for 8–16 samples.

The hybridisation reaction requires equal DNA inputs from each sample to be combined in an 8-sample pool. For each pool, carry out one hybridisation capture. The hybridisation is best performed with the maximum possible input per sample, up to 500 ng. For library yields below 500 ng, adjust the input of all samples down to the lowest yield in the hybridisation pool.

1. Use the OGT MRD Library Preparation worksheet provided to calculate the volumes of Pre-capture PCR product required to combine eight libraries to form a hybridisation pool.



Do not use inputs less than 300 ng per sample; contact [OGT Support](#) for further help.

## Library preparation: Universal hybridisation

- Aliquot 300 ng–500 ng of each of the eight libraries in a strip into a single 1.5 ml LoBind tube (see Figure 7).

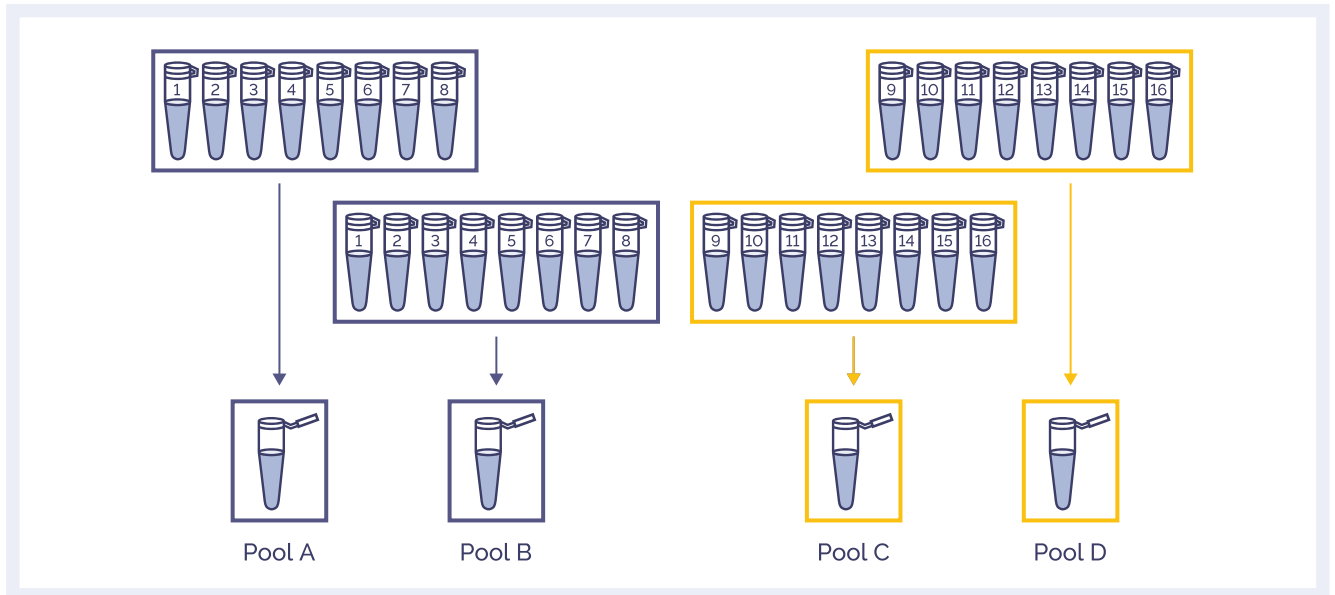


Figure 7: Pooling guide to pool 16 samples in four pools, each consisting of one strip of eight libraries.

- Add **10 µl** of Cot Human DNA (green lid; ●) to each pool.
- Mix on a vortex mixer and pulse spin to collect the contents.




Prior to use, mix beads on a vortex mixer for at least 1 min or until the bead solution appears homogeneous and consistent in colour.

- Add **2 x** volume Mag-Bind TotalPure NGS beads from the Post-PCR Universal Bead Kit to each pool.  
Example: To a 60 µl pool (+ 10 µl Cot Human DNA) add 140 µl beads.
- Mix on a vortex mixer and pulse spin to collect the contents.
- Incubate at room temperature for **5 min**.




- Place the tubes in the magnetic stand and wait for the solution to clear (approx. 3–5 min).
- Avoiding the bead pellet, remove and discard the cleared supernatant.  
**Keep the beads containing the DNA sample.**





## Library preparation: Universal hybridisation

-  10. Add **500 µl** of 80% ethanol to each tube without resuspending the bead pellet.
- 11. Incubate for **30 sec**, then remove the ethanol.
- 12. Dry the bead pellet for **approx. 5 min** or until the residual ethanol completely evaporates.



Do not over-dry as this will decrease yield. The bead pellet is dry when the appearance of the surface changes from shiny to matt. Over-drying results in cracks in the bead pellet.

- 13. Remove from the magnetic stand and add **13.5 µl** of the Hybridisation Master Mix directly to the bead pellet to elute the pooled DNA libraries. Mix on a vortex mixer to resuspend the beads and pulse spin to collect the contents.





Make sure beads are resuspended well. Larger volumes of beads might have to be vortexed longer to ensure complete resuspension.

- 14. Incubate for **5 min** at room temperature.
- 15. Label a new set of PCR strip-tubes for the pools and set aside until required in Step 17.



Recommendation: Program the thermal cycler using the settings shown in Table 9. Save the program as "OGT Hybridisation".

-  16. Place the tubes on the magnetic stand and wait for the solution to clear (approx. 2–3 min).
- 17. Transfer **13 µl** of the eluate to the empty tubes from Step 15. Tubes containing beads can be discarded at this time.
- 18. Add **2 µl** of Index Blockers (blue lid; ●) to the pools.
- 19. Add **2 µl** of SureSeq Myeloid MRD Panel to the pools.
- 20. Seal the tubes, mix on a vortex mixer and pulse spin to collect the contents. The final volume should be **17 µl**.
- 21. Make sure all caps are tightly sealed.



## Library preparation: Universal hybridisation

22. Place the tubes into the thermal cycler and run the program “OGT Hybridisation” shown in Table 8. Where possible, set the heated lid to 105°C, alternatively, have the pre-set heated lid activated.


Step	Temperature (°C)	Time
1	95	5 min
2	65	Hold

Table 8: Incubation profile of program “OGT Hybridisation”.

23. Incubate the hybridisation mixture overnight (**16–20 hr**) at 65°C.
24. Continue to “Universal capture and wash”.




Remove the Hyb Wash Buffer (blue dot; ●) and Bead Priming Buffer (orange dot; ●) from storage (–15°C to –25°C) and allow to thaw to room temperature. These can be left on the bench overnight to defrost.



## Library preparation: Universal capture and wash

### Universal capture and wash

#### Overview

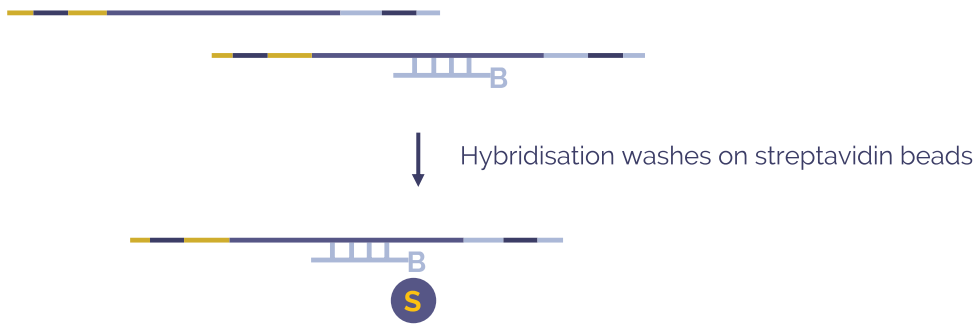

*The hybridised targets are bound to streptavidin beads and washed to remove any off-target DNA.*

Estimated time: 1.25 hr for 8–16 samples. Hands-on time: 45 min.


#### Before starting:

- Pre-warm a thermal cycler to 65°C for at least **30 min before use**.
- Pre-warm a thermal cycler to 35°C for at least **30 min before use**.



It is important to maintain the correct temperature; it is recommended that you verify the temperature using a calibrated thermometer.

- Take the Dynabeads M-270 Streptavidin magnetic beads from the Post-PCR Universal Bead Kit out of the fridge at least **30 min before use** to allow them to warm to room temperature.
- Remove the Hyb Wash Buffer (blue dot; ●) and Bead Priming Buffer (orange dot; ●) from storage (–15°C to –25°C) and allow to thaw to room temperature. These can be left on the bench overnight to defrost.



## Library preparation: Universal capture and wash

### Prepare sequence capture and bead wash buffers

1. Ensure the Hyb Wash Buffer and Bead Priming Buffer are fully thawed.



Incubate at 37°C for 5–10 min to resuspend any precipitates. It is possible to defrost these buffers at room temperature during your overnight incubation.

2. Aliquot **6 x 200 µl** of Hyb Wash Buffer per hybridisation pool into PCR strip-tubes as shown in Figure 8 for one hybridisation pool.
3. Pre-warm the aliquots to the following temperatures in a heat block for a minimum of **30 min before use**:
  - 3 x 200 µl at 65°C / pool
  - 3 x 200 µl at 35°C / pool

Pool 1	Pool 1
W1 ●	W1 ●
W2 ●	W2 ●
W3 ●	W3 ●
65°C washes	35°C washes

Figure 8: Set-up of Hyb Wash Buffer aliquots for one hybridisation pool.


### Prepare magnetic beads

1. Vortex the Dynabeads M-270 Streptavidin magnetic beads well for 1 min, changing the orientation of the tubes **every 15 seconds**.



Ensure the bead cake is completely free from the bottom or sides of the tube as addition of excess of beads will negatively impact downstream processes. Do not pulse spin the magnetic beads after mixing.

2. Immediately before use, resuspend the room temperature Dynabeads M-270 Streptavidin magnetic beads using a **200 µl** pipette set to **100 µl** and pipette mixing up and down at least **10 times**.



## Library preparation: Universal capture and wash

3. Add **100 µl** of the Dynabeads M-270 Streptavidin magnetic beads to a new PCR tube; one per hybridisation pool.



Alternatively: Up to 400 µl of beads (for four hybridisation pools) can be washed at once in a single 1.5 ml LoBind tube.




4. Place the tube(s) on a magnetic stand and wait for the solution to clear (approx. 10 sec).
5. Avoiding the bead pellet, remove and discard the cleared supernatant (~**100 µl**).
6. Add **200 µl** of 1x Bead Priming Buffer per **100 µl** beads. Mix on a vortex mixer and pulse spin to collect the contents.
7. Place the tube(s) back on the magnetic stand and wait for the solution to clear (approx. 10 sec).
8. Avoiding the bead pellet, remove and discard the cleared supernatant (~**200 µl**).
9. Repeat Steps 6–8 once, for a total of **two** washes.
10. Remove from the magnetic stand and add 1x the original volume of Bead Priming Buffer (i.e., for 100 µl of beads add 100 µl of Bead Priming Buffer), mix on a vortex mixer and pulse spin to collect the contents.
11. If washing more than 100 µl of beads per tube, label a new set of PCR strip-tubes and transfer the beads into the new PCR tubes (100 µl/pool).



12. Place the tubes on a magnetic stand, allow the beads to separate from the supernatant, then carefully remove and discard the supernatant.



Proceed immediately to "Perform hybrid capture". Do not allow the beads to dry out. Small amounts of residual Bead Priming Buffer will not interfere with the downstream binding of the DNA to Dynabeads M-270 Streptavidin magnetic beads.



## Library preparation: Universal capture and wash

### Perform hybrid capture

1. After the overnight incubation, keep the hybridised samples on the thermal cycler and transfer all the hybridised sample (~17  $\mu$ l volume) to the prepared streptavidin beads.
2. Mix thoroughly on a vortex mixer for **3–5 sec** and ensure that the beads are resuspended. Pulse spin to collect the contents.
3. Return the tubes to the thermal cycler still running program “OGT Hybridisation” at 65°C for **45 min**.
4. **Every 15 min**, mix on a vortex mixer for **3 sec** followed by a brief pulse spin to collect the contents. This ensures the beads remain in suspension. Place the tubes back in a thermal cycler running program “OGT Hybridisation”.
5. After the 45 min incubation, remove the tubes from the thermal cycler and pulse spin to collect the contents. **Proceed immediately** to the next step “Wash streptavidin beads to remove unbound DNA”.



Keep the thermal cycler program “OGT Hybridisation” running.

### Wash streptavidin beads to remove unbound DNA




Work quickly to ensure the temperature does not drop much below 65°C. To achieve this, we recommend performing all washes in PCR strip-tubes and using a multichannel pipette.



After the addition of fresh buffer, ensure the pellet has been fully resuspended by a brief mix on a vortex mixer followed by visual inspection. Do not use a pipette for mixing.

## Library preparation: Universal capture and wash

## Hot 65°C washes

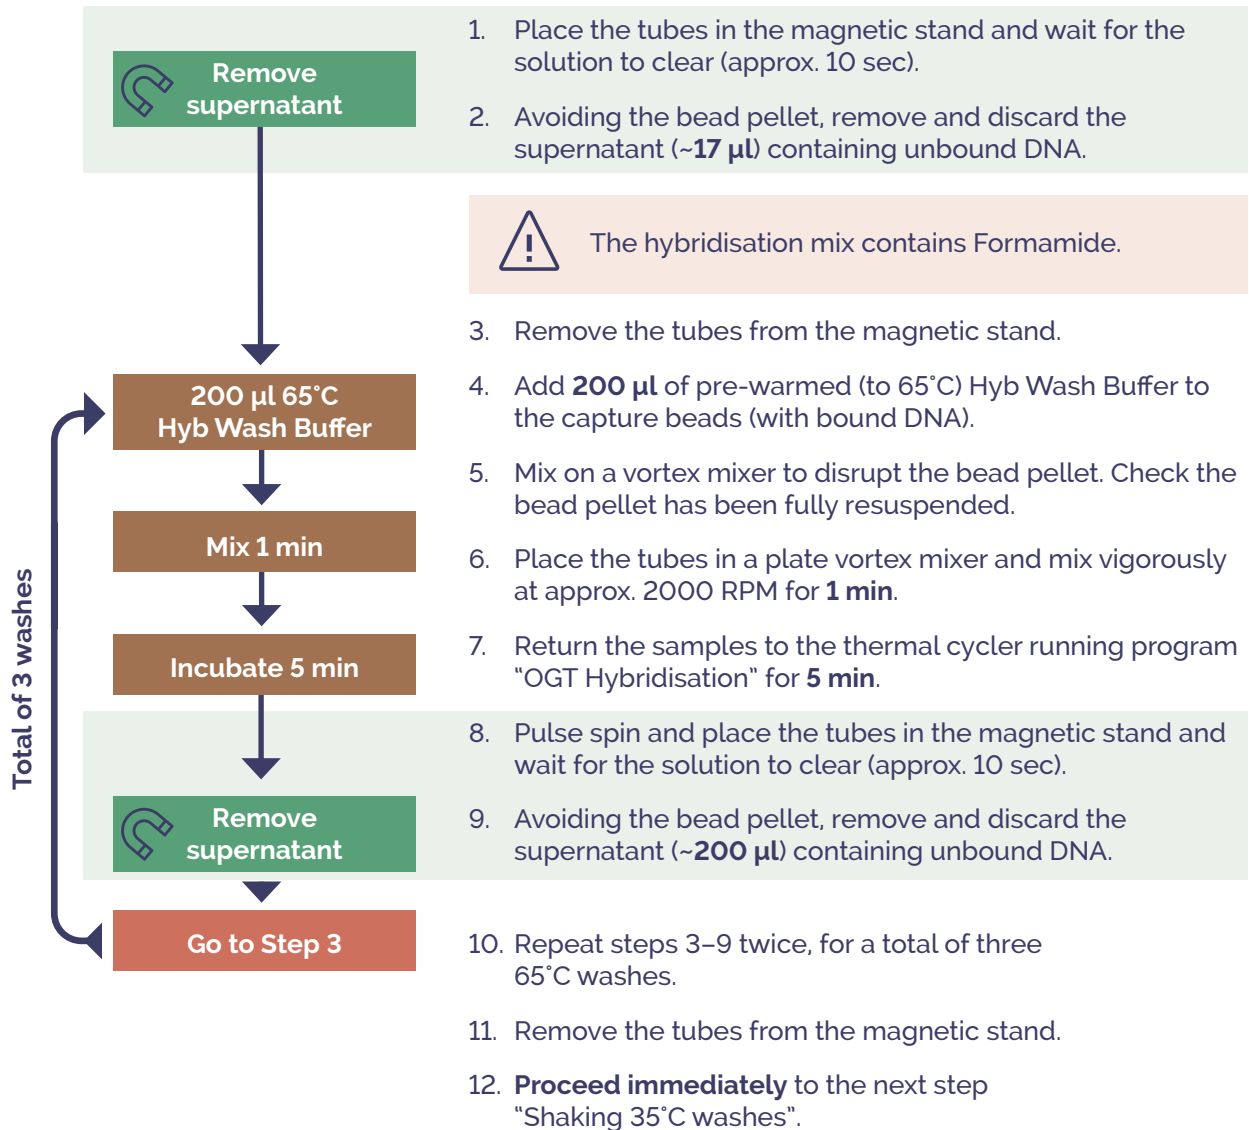

## Library preparation: Universal capture and wash

### Shaking 35°C washes

200 µl 35°C  
Hyb Wash Buffer

Mix 2 min



Remove  
supernatant

200 µl 35°C  
Hyb Wash Buffer

Mix 1 min



Remove  
supernatant

200 µl 35°C  
Hyb Wash Buffer

1. Add **200 µl** of pre-warmed (to 35°C) Hyb Wash Buffer to the capture beads.
2. Mix on a vortex mixer to disrupt the bead pellet. Check the bead pellet has been fully resuspended.
3. Place the tubes in a plate vortex mixer and mix vigorously at approx. 2000 RPM for **2 min**.
4. Pulse spin to collect the contents.
5. Place the tubes in the magnetic stand and wait for the solution to clear (approx. 10 sec).
6. Avoiding the bead pellet, remove and discard the supernatant containing unbound DNA (~**200 µl**).
7. Add **200 µl** of pre-warmed (to 35°C) Hyb Wash Buffer to the capture beads.
8. Mix on a vortex mixer to disrupt the bead pellet. Check the bead pellet has been fully resuspended.
9. Place the tubes in a plate vortex mixer and mix vigorously at approx. 2000 RPM for **1 min**.
10. Pulse spin to collect the contents.
11. Place the tubes in the magnetic stand and wait for the solution to clear (approx. 10 sec).
12. Avoiding the bead pellet, remove and discard the supernatant containing unbound DNA (~**200 µl**).
13. Add **200 µl** of pre-warmed (to 35°C) Hyb Wash Buffer to the capture beads.



## Library preparation: Universal capture and wash

## Shaking 35°C washes (continued)

Mix 30 sec

14. Mix on a vortex mixer to disrupt the bead pellet. Check the bead pellet has been fully resuspended.
15. Place the tubes in a plate vortex mixer and mix vigorously at approx. 2000 RPM for **30 sec**.



Do not mix for more than 30 sec.



Remove supernatant

16. Pulse spin to collect the contents.
17. Place the tubes in the magnetic stand and wait for the solution to clear (approx. 10 sec).
18. Avoiding the bead pellet, remove and discard the supernatant (~200 µl).
19. Pulse spin to collect the residual wash buffer. Return the tubes to the magnetic stand and remove the residual wash buffer with a P20 pipette.

Add 30 µl NFW and mix


20. Remove the tubes from the magnetic stand and add **30 µl** of Nuclease-free Water to resuspend the bead pellet.
21. Mix on a vortex mixer to form bead slurry.



Recommendation: If proceeding with Step 4: Post-capture PCR immediately, the Step 4: Primer Mix and Step 4: PCR Buffer can be removed from storage to thaw to room temperature now.




**OPTIONAL STOPPING POINT:** If the samples are not to be used immediately, store the bead slurry at 4°C. Do not freeze the bead slurry. If continuing, proceed to "Post-capture PCR".



## Library preparation: Step 4

### Post-capture PCR


#### Overview

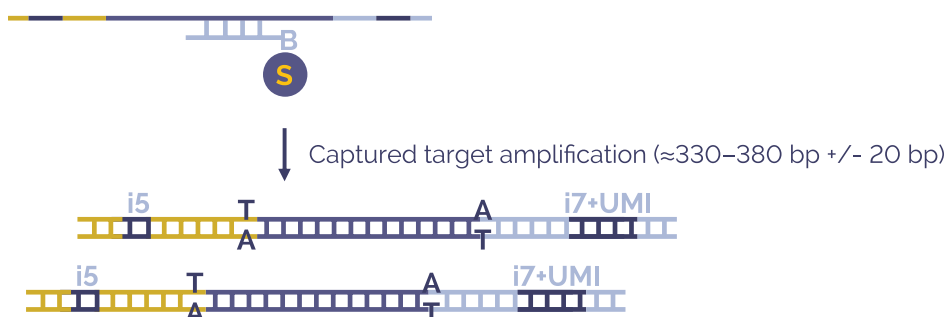

After capture of target sequences, ssDNA bound to the Streptavidin beads (S) are amplified.

#### Before starting:

- Take the Mag-Bind TotalPure NGS beads from the Post-PCR Universal Bead Kit out of the fridge at least **30 min before use** to allow them to warm to room temperature.
- Make up a fresh solution of 80% ethanol using molecular biology grade ethanol and molecular biology grade water.
- Remove the Step 4: Primer Mix (purple lid; ●) and Step 4: PCR Buffer (purple lid; ●) from storage (–15°C to –25°C) and allow to thaw at room temperature.
- Ensure that all components in the PCR Buffer are dissolved. If necessary, vortex mix and/or incubate at 37°C until dissolved.
- ❄ • Remove the Step 4: PCR Polymerase (purple lid; ●) from storage (–15°C to –25°C) and place on ice.



## Library preparation: Step 4

### Perform step 4: Post-capture PCR



To preserve sample complexity use all of the bead slurry. Two PCRs are performed on each pool.

Estimated time: 1.25 hr for 8–16 samples. Hands-on time: 15 min.

1. Program the thermal cycler using the settings shown in Table 9. Save the program as “OGT PCR2”. Where possible, set the heated lid to 105°C, alternatively have the pre-set heated lid activated.

Step	Temperature (°C)	Time
1	98	3 min
2	98	30 sec
3	65	30 sec
4	72	1 min
5	Repeat Step 2 to Step 4 for a total number of 20 cycles	
6	72	10 min
7	4	Hold

Table 9: Incubation profile of program “OGT PCR2”.

2. Mix Step 4: Primer Mix and Step 4: PCR Buffer on a vortex mixer for **3–5 sec** and pulse spin to collect the contents.
- ❄️ 3. Flick mix Step 4: PCR Polymerase, pulse spin to collect the contents and keep on ice.
4. For multiple pools, prepare the Post-capture PCR Master Mix according to Table 10 in a fresh 1.5 ml LoBind tube. There will be two PCRs prepared for each hybridisation capture pool.

## Library preparation: Step 4

Reagent	1x Pool (µl)	2x Pool (µl) 4 PCRs (includes 1 excess)	4x Pool (µl) 8 PCRs (includes 1 excess)
Captured cDNA in bead slurry	14	–	–
Nuclease-free Water	26.5	132.5	238.5
Step 4: PCR Buffer (purple lid; ●)	5	25	45
Step 4: Primer Mix (purple lid; ●)	2.5	12.5	22.5
Step 4: PCR Polymerase (purple lid; ●)	2	10	18
<b>TOTAL</b>	<b>50</b>	<b>180</b>	<b>324</b>

Table 10: Post-capture PCR Master Mix.


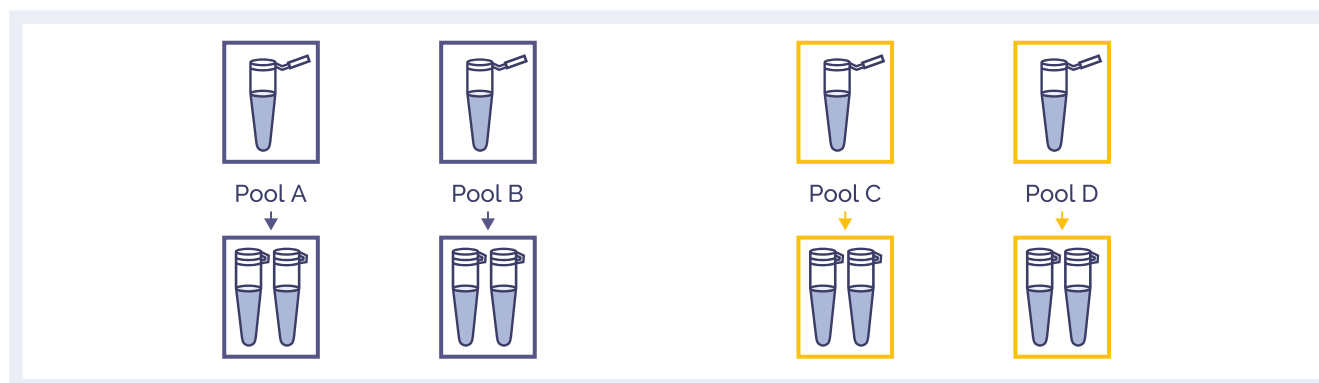


Figure 9: Post-capture PCR guide for 16 samples (4 pools). Duplicate reactions set up for each capture pool for a total of 8 PCRs.

- Mix the Post-capture PCR Master Mix on a vortex mixer for **3–5 sec** and pulse spin to collect the contents.
- Label two new PCR tubes for each hybridisation capture.
- Add **36 µl** of the Post-capture PCR Master Mix into the tubes from Step 6.
- Immediately** add **14 µl** of well-mixed bead slurry to each of the tubes prepared in Step 6.
- Ensure two PCRs are performed for each pool (see Figure 9)
- Pipette mix at least 10 times.
- Transfer to the thermal cycler and start the program “OGT PCR2”.



## Library preparation: Step 4


### Perform post-capture PCR purification

Estimated time: 40 min for 8–16 samples.



Prior to use, mix beads on a vortex mixer for at least 1 min or until the bead solution appears homogeneous and consistent in colour.

#### To the DNA sample tubes:

1. Add **45 µl** of homogeneous, room temperature Mag-Bind TotalPure NGS beads from the Post-PCR Universal Bead Kit to each DNA sample tube. Mix on a vortex mixer to resuspend the beads and pulse spin to collect the contents.
2. Incubate at room temperature for **5 min**.
-  3. Place the tubes in the magnetic stand and wait for the solution to clear (approx. 3–5 min).
4. Avoiding the bead pellet, remove and discard the cleared supernatant (**~95 µl**). **Keep the beads containing the DNA sample.**
5. Add **200 µl** of 80% ethanol to each tube without resuspending the bead pellet.
6. Incubate for **30 sec**, then remove the ethanol.
7. Repeat wash (Steps 5 and 6) once, for a total of two washes.
8. Seal the tubes and pulse spin to collect the residual ethanol. Return the tubes to the magnetic stand for **30 sec**. Remove the residual ethanol with a P20 pipette.
9. Dry the bead pellets at room temperature for **1–2 min**.



Do not over-dry as this will decrease yield. The bead pellet is dry when the appearance of the surface changes from shiny to matt. Over-drying results in cracks in the bead pellet.

10. Remove from the magnetic stand and add **22 µl** of Nuclease-free Water directly to the bead pellet to elute the DNA sample. Mix on a vortex mixer and pulse spin to collect the contents.
11. Incubate for **5 min** at room temperature.

## Library preparation: Step 4

12. Label a new set of PCR strip-tubes for the eluates and set aside until required in Step 14.



13. Place the tubes on the magnetic stand and wait for the solution to clear (approx. 2–3 min).

14. Transfer **20 µl** of the eluate containing the purified post-capture PCR products to the tubes from Step 12. The tubes containing beads can be discarded at this time.

15. Assess the size of the amplified product using the Agilent High Sensitivity D1000 ScreenTape System. The electropherogram should show a maximum peak size of 330–350 bp (+/- 20 bp) (Figure 10). Set up the instrument and prepare the tape, samples and ladder following the manufacturer's instructions.


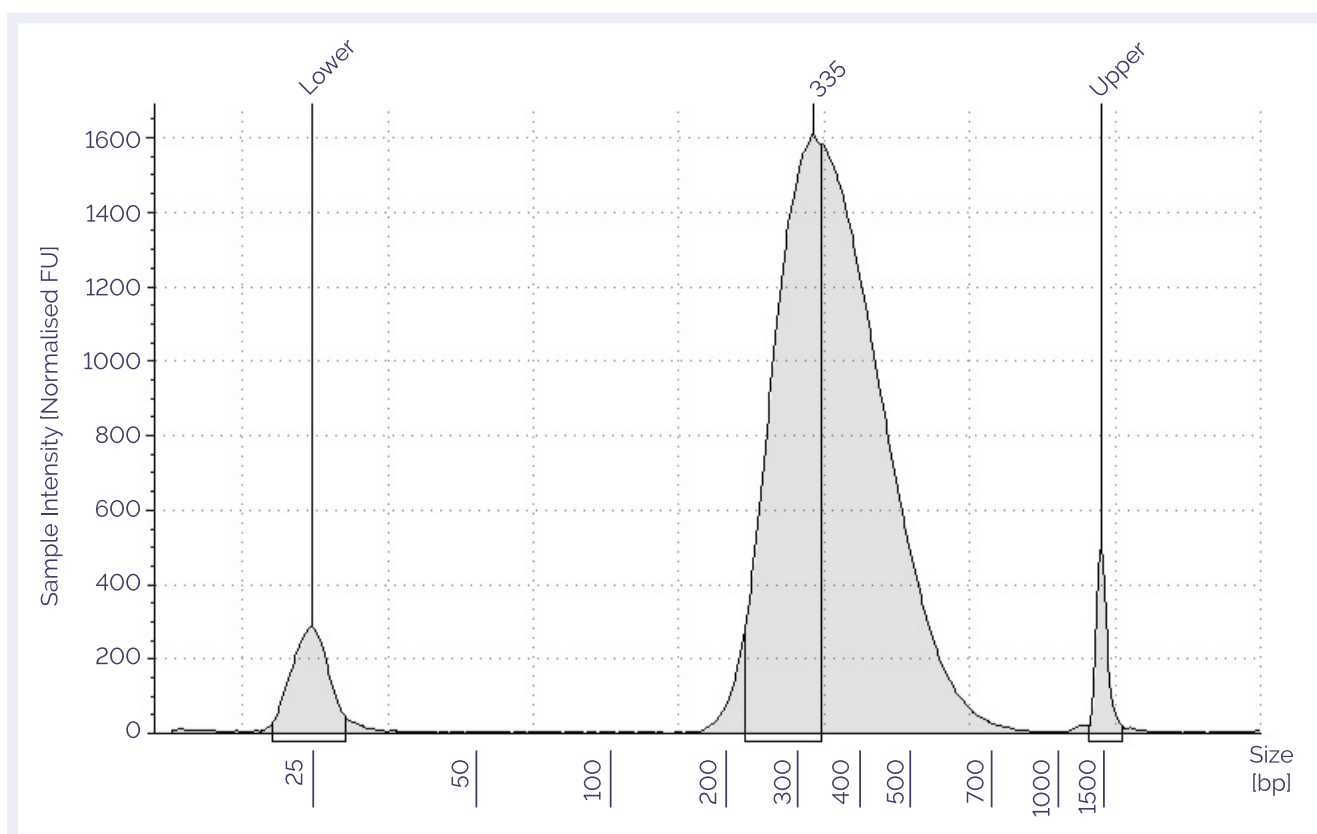


Figure 10: Electropherogram of purified Post-capture PCR product generated using an Agilent High Sensitivity D1000 ScreenTape assay. The electropherogram shows a maximum peak in the size range of approximately 330–350 bp (+/- 20 bp).



## Library preparation: Step 4



Fragment sizes outside of this range may reduce sequence data quality. Contact your local Field Application Specialist (FAS) for further details.

- Assess yield using **1  $\mu$ l** amplified product with the Qubit dsDNA HS Kit as per manufacturer's instructions. The expected yield is 5–15 ng/ $\mu$ l.



**OPTIONAL STOPPING POINT:** If the samples are not to be used immediately, store them at 4°C overnight or at –20°C for long-term storage. If continuing, proceed to “Sequencing”.

## Sequencing

### Sequencing

#### Overview

The DNA capture pools prepared in the previous section (Post-capture PCR) need to be combined such that each pool is present in equimolar amounts when loaded onto the sequencer. This requires both accurate determination of peak size (bp), provided by Agilent TapeStation (High Sensitivity Kit), and accurate determination of sample concentration (ng/ $\mu$ l), provided by Thermo Fisher Scientific Qubit (High Sensitivity) assay.

#### Preparing the sequencing pool




A worksheet can be created using the “OGT\_ULPK\_Worksheet” template provided by OGT. Alternatively use the formulae below.

- Use your worksheet described above or the formulae below to determine the volume ( $\mu$ l) of each DNA capture pool required to generate the 4 nM sequencing pool.



This protocol has been validated with 150-base paired-end reads using the NextSeq 550 High-Output Kit 2x150bp (Illumina cat. no. 20024908).



## Sequencing

2. Complete the “Sequencing Pool Parameters” and “Samples” tables in the “PCR2” tab of the pooling template. Cells in green should be manually modified as required; parameters marked with \* must be provided.
3. Add the appropriate volume of each indexed sequencing pool to a fresh 1.5 ml LoBind tube labelled “4 nM Sequencing Pool”; the volumes can be found in the column labelled “Volume of PCR2 product to pipette” in the “Volumes to pipette” tabs.
4. Adjust the final volume of the sequencing pool with Nuclease-free Water to the desired final concentration (4 nM). This can be found in Column B of the “Volumes to pipette” tabs next to “Volume of Nuclease-free water to pipette”.
5. Validation of sequencing pool concentration: Assess peak size distribution of the sequencing pool using the Agilent High Sensitivity D1000 ScreenTape System; and assess yield using the Qubit dsDNA HS Kit. Complete the “Pool validation and dilution” tab to determine the molar concentration of the sequencing pool.
6. The sequencing pool is ready for loading on to the sequencer.



**OPTIONAL STOPPING POINT:** If the sequencing pool is not to be used immediately, store at -20°C for long-term storage. If continuing, proceed to “Preparing the Sample Sheet”.

### Formula 1 — nM of each sample

$$nM = \frac{[\text{Sample concentration (ng/}\mu\text{l)}] \times 10^6}{([\text{Sample size in bp}] \times 660) + 157.9}$$

### Formula 2 — volume of each indexed DNA sample

$$\text{Volume of indexed sample} = \frac{\text{Sequencing Pool } (\mu\text{l}) \times \text{Pool concentration (4 nM)}}{\text{Number of samples in Pool} \times \text{nM concentration of the sample}}$$



## Sequencing

### Preparing the Sample Sheet



A NextSeq Sample Sheet can be created using the NextSeq pooling guide provided by OGT.

1. Open the completed Worksheet and click on the relevant Sample Sheet tab.




This sheet will be automatically filled with the parameters and sample data entered into the "PCR1" and "PCR2" sheets.

2. Highlight all cells with text as shown in Figure 10. Adjust the number of rows highlighted as appropriate.

[Header]									
1	[Header]								
2	IEMFileVersion		4						
3	Investigator Name	xxx							
4	Project Name	xxx							
5	Experiment Name	xxx							
6	Date	DD/MM/YYYY							
7	Workflow	GenerateFASTQ							
8	Application	FASTQ Only							
9	Assay	OGT_enrichment							
10	Description								
11	Chemistry	Amplicon							
12									
13	[Reads]								
14		150							
15		150							
16									
17	[Settings]								
18	ReverseComplement		0						
19									
20									
21									
22									
23	[Data]								
24	Sample_ID	Sample_Name	Sample_Plate	Sample_Well	I7_Index_ID	index	I5_Index_ID	index2	Sample_Project
25	A1	A1			73	GTTGACCTNNNNNNNNNN	573	AAGCACTG	xxx
26	B1	B1			74	CGTGTGTANNNNNNNNNN	574	TCGTTGG	xxx
27	C1	C1			75	ACGACTTGNNNNNNNNN	575	TCGCTGT	xxx
28	D1	D1			76	CAGTACTNNNNNNNNNN	576	GAATCCGA	xxx
29	E1	E1			77	ACTAGGAGNNNNNNNNNN	577	GTGCCATA	xxx
30	F1	F1			78	GTAGGAGTNNNNNNNNNN	578	CTTAGGAC	xxx
31	G1	G1			79	CCTGATTGNNNNNNNNN	579	AACTGAGC	xxx
32	H1	H1			80	ATGCACGANNNNNNNNNN	580	GACGATCT	xxx
33	A2	A2			81	CGACTTTANNNNNNNNNN	581	ATCCAGAG	xxx
34	B2	B2			82	TACGCTTNNNNNNNNNN	582	AGAGTAGC	xxx
35	C2	C2			83	CCGTAAGANNNNNNNNNN	583	TGGACTCT	xxx
36	D2	D2			84	ATCACAGNNNNNNNNNN	584	TACGCTAC	xxx
37	E2	E2			85	CACCTGTTNNNNNNNNNN	585	GCTATCCT	xxx
38	F2	F2			86	CTTCGACTNNNNNNNNNN	586	GCAAGATC	xxx
39	G2	G2			87	TGCTCCANNNNNNNNNN	587	ATCGATCG	xxx
40	H2	H2			88	AGAAGCAGNNNNNNNNNN	588	CGGCTAAT	xxx

Figure 11: Example Sample Sheet on the NextSeq pooling template.



## Sequencing

- Copy highlighted cells and paste into a new Excel file.



All text in red is for user and sample specific information. All text in black is required to ensure that the sequencer will recognise the file.

- Save the new sheet as a CSV (comma delimited) file.
- The Sample Sheet can now be uploaded to the sequencer.



**OPTIONAL STOPPING POINT:** If the sequencing pool is not to be used immediately, store at  $-20^{\circ}\text{C}$  for long-term storage. If continuing, proceed to "Denaturing and loading the sequencing pool" or refer to the appropriate Illumina protocol.

## Denaturing and loading the sequencing pool

- Follow the appropriate Illumina protocol for denaturing the sequencing pool.



If the sequencer has only one dilution step, follow the Illumina protocol for loading. If the sequencer requires a secondary dilution step, for example the dilution of the 20 pM Denatured pool to a 1.4 pM Loading pool on a NextSeq, continue with Step 2.



- Make the volume of the pool up to 1 ml with ice-cold HT1 to dilute your denatured pool to  $\sim 20$  pM and keep on ice.



Volumes of HT1 required will vary depending on the volume of Denatured pool, dictated by the sequencer type. The actual concentration of the  $\sim 20$  pM pool can be found on the "Pool validation and dilution" tab in the worksheet and will depend on the concentration of the sequencing pool.

- Enter the required sequencer loading concentration into the "Pool validation and dilution" tab in your worksheet.




Cluster density can vary between machines. We recommend loading a final concentration of 1.4 pM if using a NextSeq 500/550 High-Output Kit.

- Dilute the denatured 20 pM pool to this loading concentration by pipetting the volumes stated in the "Pool validation and dilution" tab in your worksheet.



If running a NextSeq, the sequencing pool should be combined with 5% denatured PhiX before running, according to the Illumina protocol.



## Sequencing

5. Pipette the loading pool into the sequencer cartridge and set up the sequencing run according to the Illumina protocol.
6. If using BaseSpace, select “+ Custom Library Prep Kit” in the Library Prep Kit dropdown menu.
7. Use the information in Table 13 in the Appendix to create the “Universal NGS Library preparation kit”.
8. The “Universal NGS Library preparation kit” will now be available to use for the sequencing run.

## Appendix


### Adapter sequences

Adapter	Sequence
1	AGATCGGAAGAGCACACGTCTGAACTCCAGTCA
2	AGATCGGAAGAGCGTCGTGTAGGGAAAGAGTGT

Table 11: Adapter sequences – forward configuration. Please note some Illumina sequencing instruments require the reverse complement of the Index 2 (i5) Adapter sequence.


### Index sequences

I7_Index_ID	Index 1 sequence	I5_Index_ID	Index 2 sequence
1	CTGATCGTNNNNNNNNNN	501	ATATGCGC
2	ACTCTCGANNNNNNNNNN	502	TGGTACAG
3	TGAGCTAGNNNNNNNNNN	503	AACCGTTC
4	GAGACGATNNNNNNNNNN	504	TAACCGGT
5	CTTGTCGANNNNNNNNNN	505	GAACATCG
6	TTCCAAGGNNNNNNNNNN	506	CCTTGTAG
7	CGCATGATNNNNNNNNNN	507	TCAGGCTT




## Appendix

I7_Index_ID	Index 1 sequence	I5_Index_ID	Index 2 sequence
8	ACGGAACANNNNNNNNNN	508	GTTCTCGT
9	CGGCTAATNNNNNNNNNN	509	AGAACGAG
10	ATCGATCGNNNNNNNNNN	510	TGCTTCCA
11	GCAAGATCNNNNNNNNNN	511	CTTCGACT
12	GCTATCCTNNNNNNNNNN	512	CACCTGTT
13	TACGCTACNNNNNNNNNN	513	ATCACACG
14	TGGACTCTNNNNNNNNNN	514	CCGTAAGA
15	AGAGTAGCNNNNNNNNNN	515	TACGCCTT
16	ATCCAGAGNNNNNNNNNN	516	CGACGTTA
17	GACGATCTNNNNNNNNNN	517	ATGCACGA
18	AACTGAGCNNNNNNNNNN	518	CCTGATTG
19	CTTAGGACNNNNNNNNNN	519	GTAGGAGT
20	GTGCCATANNNNNNNNNN	520	ACTAGGAG
21	GAATCCGANNNNNNNNNN	521	CACTAGCT
22	TCGCTGTTNNNNNNNNNN	522	ACGACTTG
23	TTCGTTGGNNNNNNNNNN	523	CGTGTGTA
24	AAGCACTGNNNNNNNNNN	524	GTTGACCT
25	CCTTGATCNNNNNNNNNN	525	ACTCCATC
26	GTCGAAGANNNNNNNNNN	526	CAATGTGG
27	ACCACGATNNNNNNNNNN	527	TTGCAGAC
28	GATTACCGNNNNNNNNNN	528	CAGTCCAA
29	GCACAACNNNNNNNNNN	529	ACGTTCCAG
30	GCGTCATTNNNNNNNNNN	530	AACGTCTG
31	ATCCGGTANNNNNNNNNN	531	TATCGGTC




## Appendix

I7_Index_ID	Index 1 sequence	I5_Index_ID	Index 2 sequence
32	CGTTGCAANNNNNNNNNN	532	CGCTCTAT
33	GTGAAGTGNNNNNNNNNN	533	GATTGCTC
34	CATGGCTANNNNNNNNNN	534	GATGTGTG
35	ATGCCTGTNNNNNNNNNN	535	CGCAATCT
36	CAACACCTNNNNNNNNNN	536	TGGTAGCT
37	TGTGACTGNNNNNNNNNN	537	GATAGGCT
38	GTCATCGANNNNNNNNNN	538	AGTGGATC
39	AGCACTTCNNNNNNNNNN	539	TTGGACGT
40	GAAGGAAGNNNNNNNNNN	540	ATGACGTC
41	GTTGTTTCGNNNNNNNNNN	541	GAAGTTGG
42	CGGTTGTTNNNNNNNNNN	542	CATACCAC
43	ACTGAGGTNNNNNNNNNN	543	CTGTTGAC
44	TGAAGACGNNNNNNNNNN	544	TGGCATGT
45	GTTACGCANNNNNNNNNN	545	ATCGCCAT
46	AGCGTGTTNNNNNNNNNN	546	TTGCGAAG
47	GATCGAGTNNNNNNNNNN	547	AGTTCGTC
48	ACAGCTCANNNNNNNNNN	548	GAGCAGTA
49	GAGCAGTANNNNNNNNNN	549	ACAGCTCA
50	AGTTCGTCNNNNNNNNNN	550	GATCGAGT
51	TTGCGAAGNNNNNNNNNN	551	AGCGTGTT
52	ATCGCCATNNNNNNNNNN	552	GTTACGCA
53	TGGCATGTNNNNNNNNNN	553	TGAAGACG
54	CTGTTGACNNNNNNNNNN	554	ACTGAGGT
55	CATACCACNNNNNNNNNN	555	CGGTTGTT



## Appendix

I7_Index_ID	Index 1 sequence	I5_Index_ID	Index 2 sequence
56	GAAGTTGGNNNNNNNNNN	556	GTTGTTCCG
57	ATGACGTCNNNNNNNNNN	557	GAAGGAAG
58	TTGGACGTNNNNNNNNNN	558	AGCACTTC
59	AGTGGATCNNNNNNNNNN	559	GTCATCGA
60	GATAGGCTNNNNNNNNNN	560	TGTGACTG
61	TGGTAGCTNNNNNNNNNN	561	CAACACCT
62	CGCAATCTNNNNNNNNNN	562	ATGCCTGT
63	GATGTGTGNNNNNNNNNN	563	CATGGCTA
64	GATTGCTCNNNNNNNNNN	564	GTGAAGTG
65	CGCTCTATNNNNNNNNNN	565	CGTTGCAA
66	TATCGGTCNNNNNNNNNN	566	ATCCGGTA
67	AACGTCTGNNNNNNNNNN	567	GCGTCATT
68	ACGTTCAAGNNNNNNNNNN	568	GCACAAC
69	CAGTCCAANNNNNNNNNN	569	GATTACCG
70	TTGCAGACNNNNNNNNNN	570	ACCACGAT
71	CAATGTGGNNNNNNNNNN	571	GTCGAAGA
72	ACTCCATCNNNNNNNNNN	572	CCTTGATC
73	GTTGACCTNNNNNNNNNN	573	AAGCACTG
74	CGTGTGTANNNNNNNNNN	574	TTCGTTGG
75	ACGACTTGNNNNNNNNNN	575	TCGCTGTT
76	CACTAGCTNNNNNNNNNN	576	GAATCCGA
77	ACTAGGAGNNNNNNNNNN	577	GTGCCATA
78	GTAGGAGTNNNNNNNNNN	578	CTTAGGAC
79	CCTGATTGNNNNNNNNNN	579	AACTGAGC



## Appendix


I7_Index_ID	Index 1 sequence	I5_Index_ID	Index 2 sequence
80	ATGCACGANNNNNNNNNN	580	GACGATCT
81	CGACGTTANNNNNNNNN	581	ATCCAGAG
82	TACGCCTTNNNNNNNNN	582	AGAGTAGC
83	CCGTAAGANNNNNNNNN	583	TGGA CTCT
84	ATCACACGNNNNNNNNN	584	TACGCTAC
85	CACCTGTTNNNNNNNNN	585	GCTATCCT
86	CTTCGACTNNNNNNNNN	586	GCAAGATC
87	TGCTTCCANNNNNNNNN	587	ATCGATCG
88	AGAACGAGNNNNNNNNN	588	CGGCTAAT
89	GTTCTCGTNNNNNNNNN	589	ACGGAACA
90	TCAGGCTTNNNNNNNNN	590	CGCATGAT
91	CCTTG TAGNNNNNNNNN	591	TTCCAAGG
92	GAACATCGNNNNNNNNN	592	CTTGTCGA
93	TAACCGGTNNNNNNNNN	593	GAGACGAT
94	AACCGTTCNNNNNNNNN	594	TGAGCTAG
95	TGGTACAGNNNNNNNNN	595	ACTCTCGA
96	ATATGCGCNNNNNNNNN	596	CTGATCGT

Table 12: Index sequences. N denotes UMI. Please note, some Illumina sequencing instruments require the reverse complement of the Index 2 (i5) Adapter sequence.

## Recommended sequencing guidelines

Panel	Recommended sequencing platform	Number of samples per sequencing run	Pool size proposal	Recommended kit size purchase	Number of runs based on kit size purchase
770026-48 SureSeq Myeloid MRD Panel	NextSeq High-Output	16	4 x 8-plex	1 x 96 reactions	3 runs

Table 13: Recommended sequencing guidelines.



## Appendix

### Reagent tube locations

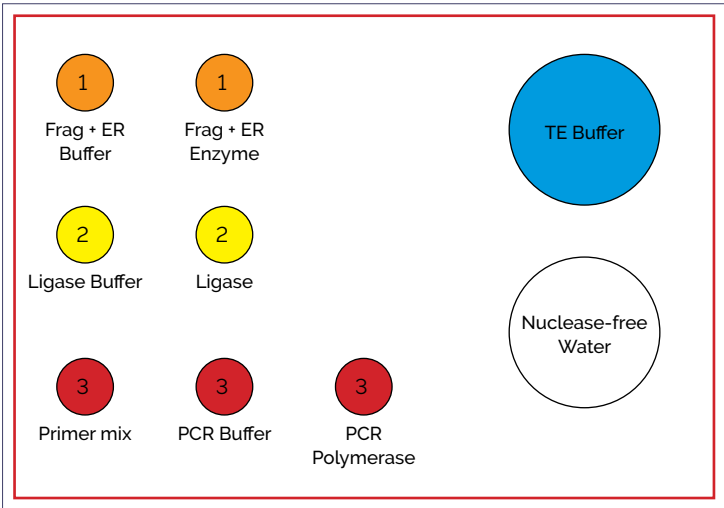


Figure 12: Location of tubes in 96 reaction Library Preparation Kit (770100-96).


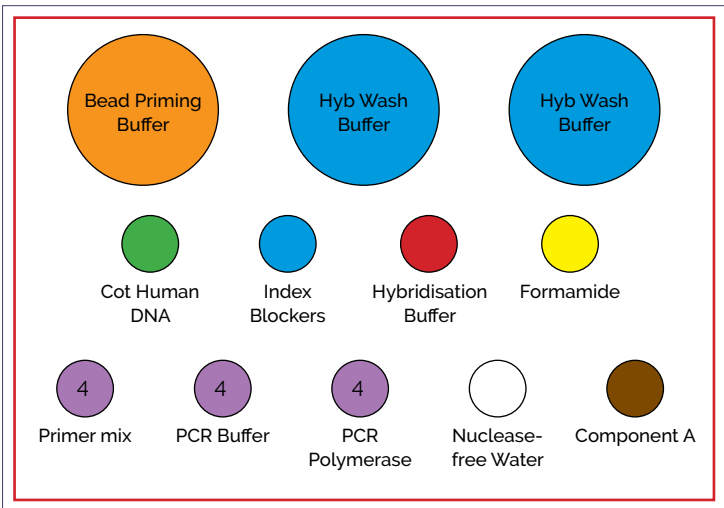


Figure 13: Location of tubes in 96 reaction Hybridisation & Wash Kit V2 (770410-96).





## Legal information

---

This handbook and its contents are © Oxford Gene Technology (Operations) Limited 2025. All rights reserved. Reproduction of all or any substantial part of its contents in any form is prohibited except that individual users may print or save portions of the protocol for their own personal use. This licence does not permit users to incorporate the material or any substantial part of it in any other work or publication, whether in hard copy or electronic or any other form. In particular (but without limitation), no substantial part of the handbook may be distributed or copied for any commercial purpose.

## NGS Library Preparation Assay

---

The Universal NGS Library Preparation Kit was developed by Oxford Gene Technology. The purchaser has the non-transferable right to use and consume the product for RESEARCH USE ONLY AND NOT FOR DIAGNOSTICS PROCEDURES. It is not intended for use, and should not be used, for the diagnosis, prevention, monitoring, treatment or alleviation of any disease or condition, or for the investigation of any physiological process, in any identifiable human, or for any other medical purpose.

## Trademarks


---

OGT™, SureSeq™, CytoSure® (Oxford Gene Technology); Agilent®, TapeStation® (Agilent Technologies Inc.); NextSeq™, NovaSeq™ (Illumina Inc.); Dynabeads™, DynaMag™, NanoDrop™, Qubit® (Thermo Fisher Scientific); IKA™, Mag-Bind® (Omega Bio-tek, Inc); LoBind® (Eppendorf SE).

## Customer's obligations

---

The Customer acknowledges that Oxford Gene Technology (Operations) Limited (or its group companies) owns all intellectual property rights in the design of the Product, including the choice and configuration of the oligonucleotide sequences used in the Product. The Product may only be reproduced or manufactured by Oxford Gene Technology (Operations) Limited or with its permission.



## Ordering information

Product	Contents	Cat. No.
Universal NGS Workflow Solution V2 (96)	Bundle of 1 x Universal Library Preparation Kit (96) containing PCR primers and enzymes, 1 x Universal Hybridisation & Wash Kit V2 (96). 1 x Pre-PCR Universal Bead Kit (96). 1 x Post-PCR Universal Bead Kit (96). 1 x Universal Index Adapter Kit (96)	770510-96

Table 14: Ordering information.

**For an up-to-date product list and the latest product information, visit [ogt.com](http://ogt.com)**

### Contact information

**UK +44 (0) 1865 856826**

**US +1 914 467 5285**

**Technical support: [support@ogt.com](mailto:support@ogt.com)**

**[contact@ogt.com](mailto:contact@ogt.com)**

**[ogt.com](http://ogt.com)**

**Oxford Gene Technology Ltd.**

**Unit 5, Oxford Technology Park, 4A Technology Drive, Kidlington, Oxfordshire, OX5 1GN, UK.**



A Sysmex Group Company

**What binds us,  
makes us.**

Oxford Gene Technology (Operations) Ltd.

Registered in England No: 03845432 Unit, 5 Oxford Technology Park, 4A Technology Drive, Kidlington, Oxfordshire, OX5 1GN, UK.

01/25

OGT SureSeq Myeloid MRD 0.05% VAF Workflow v1

For Research Use Only; Not for Use in Diagnostic Procedures